



Dhyana 400BSI V3

User Manual

V1.0.1



Copyright 2011-2024 Tucsen Photonics Co., Ltd.

All rights reserved.

Contents

1. Introduction	4
1.1. Disclaimer	4
1.2. Safety and warning information	6
2. Product specifications	8
2.1. Packaging List.....	8
2.2. Quantum efficiency curve	9
2.3. Window curve	10
2.4. Quartz window curve	10
2.5. Camera power and signal connection	11
3. Features and Functions.....	12
3.1. Camera Introduction	12
3.2. Structure and Operation of sCMOS	12
3.3. Shutter Mode	13
3.4. Front-Illuminated and Back-Illuminated sCMOS Technology.....	14
3.5. Readout Noise	15
3.6. Defective Pixel Correction (DPC).....	16
3.7. Dark Signal Non-Uniformity (DSNU)	16
3.8. Photo Response Non-Uniformity (PRNU)	17
3.9. Gain Mode	18
3.9.1. High Dynamic Range	19
3.9.2. High Sensitivity	19
3.9.3. High Speed.....	20
3.9.4. Global Reset.....	20
3.10. Region of Interest Readout.....	21
3.11. Binning Readout	22
3.12. Timestamp	24
3.13. Frame Rate Calculation.....	25
3.14. Frame Rate Adjustment.....	27
3.15. Incident Photon Calculation	27
3.16. Acquisition Mode	28
3.16.1. Live mode	28
3.16.2. Software Trigger Mode	29
3.16.3. Hardware Trigger Mode.....	29
3.16.4. Rolling Shutter Control Mode	36

3.17. Trigger Output	39
3.17.1. Hardware Trigger output circuit	39
3.17.2. Trigger Output Timing Diagram	39
3.18. Cooling.....	41
4. Installation	42
4.1. Recommended computer configurations.....	42
4.2. Camera installation.....	42
4.3. Water cooling pipe installation.....	43
4.3.1. Connect the water cooling pipe.....	43
4.3.2. Software Fan Status	44
4.3.3. Disconnect the water cooling pipe	44
4.4. Frame grabber installation	46
4.5. Driver installation and uninstallation	47
4.5.1. Camera USB driver installation	47
4.5.2. CameraLink driver installation	49
4.5.3. CameraLink driver uninstallation	50
4.6. Software installation and uninstallation.....	51
4.6.1. Installation	51
4.6.2. Uninstallation.....	53
5. Maintenance	55
5.1. Regular inspections	55
5.2. Electrical safety inspection	55
5.3. Cooling hoses and connectors	55
5.4. Basic usage	55
5.5. Window cleaning	55
6. Troubleshooting	57
6.1. The computer cannot recognize the camera.....	57
6.2. Software pauses or freezes.....	57
6.3. The camera cannot reach the target cooling temperature.....	57
6.4. The frame rate cannot reach the nominal level	57
7. FAQs	59
7.1. Why is the brightness of the captured image inconsistent with the preview window?.....	59
7.2. Stripe like flicker appears in the camera preview image	59
8. After-sales Support.....	60
Appendix 1 : Dimensions.....	61



Appendix 2 : Specifications.....	62
Appendix 3 : Third party software applications	64
Appendix 4 : Third party certification	65
Appendix 5 : Dew point table	67
Appendix 6 : Update log	68

1. Introduction

1.1. Disclaimer

To protect the legitimate rights and interests of users, please carefully read our accompanying instructions, disclaimers, and safety instructions before using our company's products. This camera user manual document contains basic information about the camera, installation instructions, product features, and maintenance, aiming to make it more convenient for users to use the TUCSEN's camera. This document is only disclosed for the above purposes. Please make sure to follow the instructions and safety instructions when operating this product.

Under no circumstances shall any content in this document constitute any express, implied, statutory or other form of warranty, including but not limited to any warranties of merchantability, non infringement or suitability for a specific purpose.

In any case, TUCSEN shall not be liable for any losses or damages arising from or related to the unauthorized use of the content of this document, whether direct, indirect, special, incidental, consequential or other reasons, whether caused by infringement or other reasons.

Product usage restrictions:

The product can only be used according to the instructions in the user manual, and unauthorized modifications, tampering, or reverse engineering are not allowed. Users are reminded that if they do not use the product according to the instructions in the user manual, resulting in product damage or malfunction, the responsibility shall be borne by the user. During the actual operation of the product, users should adjust and apply according to the content of the product manual, disclaimer, and safety instructions, combined with their own actual situation and needs. Our company does not assume any legal responsibility for any personal injury or property damage caused by users violating the product manual, disclaimer, safety instructions, or improper operation.

Quoting third-party content:





- 1) The user manual may contain content or links provided by third parties, which are for user reference and convenience only. TUCSEN only directly references the content or links of third parties and does not guarantee their authenticity, accuracy, and completeness, and does not assume any responsibility.

- 2) The publication of information in this document does not imply that TUCSEN Company or any third party automatically waives any patent or exclusive rights.
- 3) This document may contain technical or printing errors. Under no circumstances shall TUCSEN be liable for any loss or damage caused by unauthorized use of the content of this document, whether direct, indirect, special, incidental, consequential or otherwise.

Copyright and Protection Statement:

The copyright of this document and related drawings belongs to TUCSEN, and TUCSEN reserves all rights including interpretation. This document and related drawings shall not be copied, reprinted, or copied without authorization, and the relevant content shall not be disclosed without authorization.

Trademark and Patent Information:

, , ,  are trademarks of TUCSEN, and no one shall infringe upon the trademark rights of TUCSEN. All other trademarks are the property of their trademark owners, and TUCSEN is not responsible for any infringement by others.

Update of user manual:

TUCSEN does not promise to notify updates or maintain the information contained in this document at any time. If changes are made to the product, the relevant change information will be included in the new version of the manual. Without prior notice.

In summary, before using our company's products, please carefully read and understand the above disclaimer. Wishing you a pleasant use, thank you!

Tucsen Photonics Co., Ltd.

1.2. Safety and warning information

Operation and Use



Caution

- Do not drop, disassemble, repair or replace internal components on your own. Such action may damage the camera components or cause personal injury.
- In the event of spillage on the equipment, please disconnect the equipment and immediately contact the nearest dealer or manufacturer for technical assistance.
- Do not touch the device with wet hands, as it may cause electric shock.
- Do not let children touch the device without supervision.
- Ensure that the temperature of the camera is within the specified temperature range for use to avoid damage.

Installation and maintenance



Caution

- Please do not install it in dusty and dirty areas or near air conditioning or heaters to reduce the risk of camera damage.
- Avoid installation and operation in extreme environments such as vibration, high temperature, humidity, dust, strong magnetic fields, explosive/corrosive gases or gases.
- Do not apply excessive vibration and impact to the equipment. This may damage the equipment.
- Do not install equipment under unstable lighting conditions. Severe lighting changes can affect the quality of the images generated by the device, avoiding high-energy lasers directly hitting the camera chip.
- Do not use solvents or diluents to clean the surface of the equipment, as this will damage the surface of the casing.
- Please ensure that there is at least 10 cm of space around the device ventilation opening to ensure airflow flow. Do not block the ventilation openings of the equipment during use, otherwise it may cause internal temperature to be too high and damage the equipment.

Power



Caution

- Please use the original power adapter of the camera, as using an mismatched power source may damage the camera.
- If the voltage applied to the camera is greater than or less than the nominal voltage of the camera, the camera may be damaged or malfunction.
- Please refer to the specification table for the nominal voltage of the camera.

2. Product specifications

2.1. Packaging List

Standard Item Name	Specification	Quantity	Image
sCMOS scientific grade camera	Dhyana 400BSI V3	1	
Power adapter	12V/8A	1	
Power adapter power cord	Three core 250V/2.5A	1	
USB3.0 data cable	2 m	1	
USB flash drive	Software and Drivers	1	
Water pipes	2 m, OD: 6 mm, ID: 4 mm	2	
SMA trigger cable	3 m, SMA inner screw inner needle-SMA inner screw inner needle, wire RG178	4	

Optional Item Name	Specification	Quantity	Image
CameraLink frame grabber	Firebird	1	
Frame grabber cable	3 m	2	
Level conversion box	Standard	1	

2.2. Quantum efficiency curve

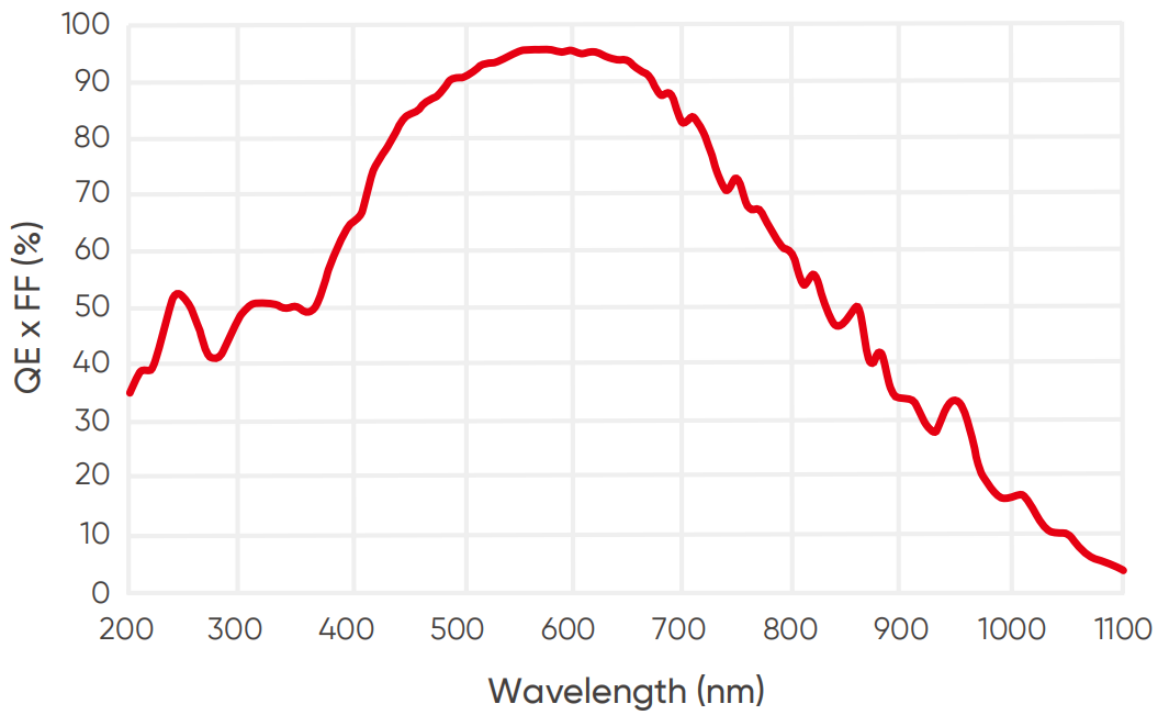


Figure 2-1 Quantum efficiency curve of Dhyana 400BSI V3

2.3. Window curve

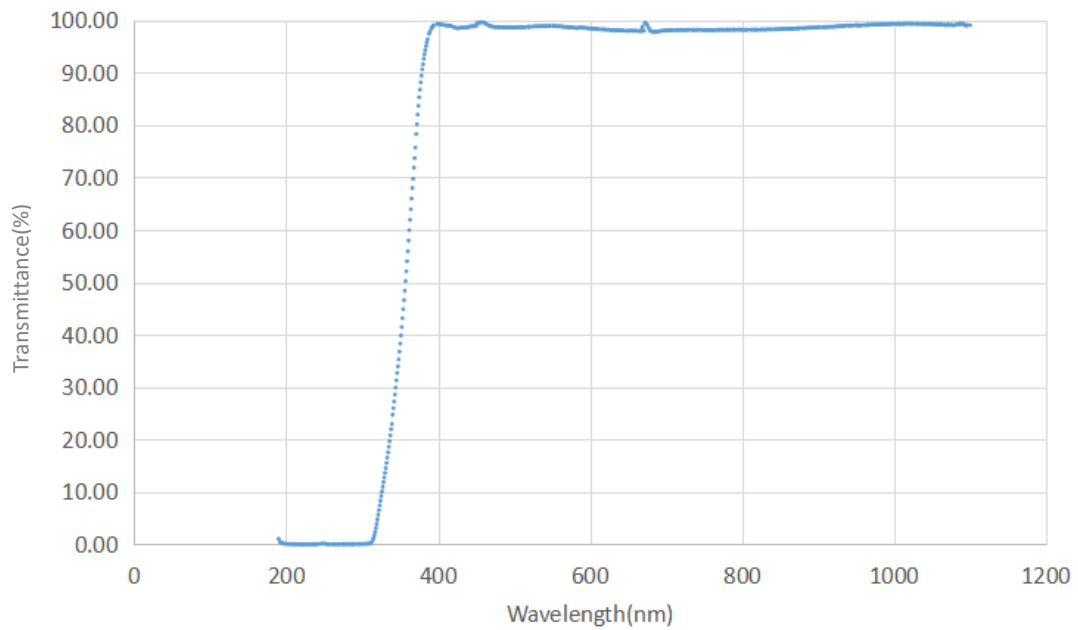


Figure 2-2 Transmission curve of a standard glass window

2.4. Quartz window curve

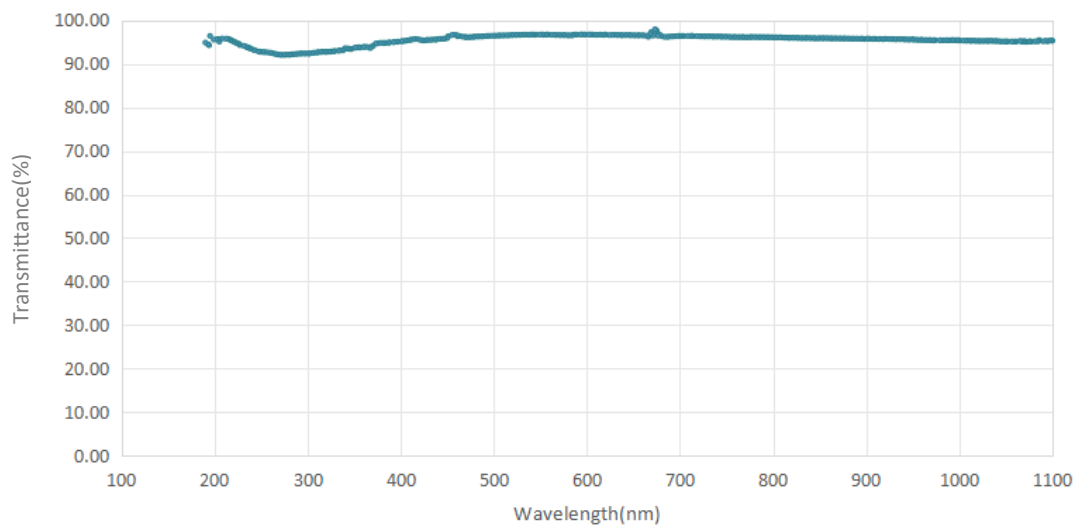


Figure 2-3 Transmission curve of a quartz window

2.5. Camera power and signal connection

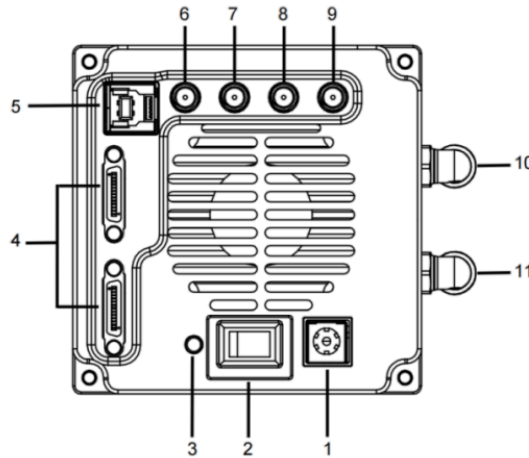


Figure 2-4 Camera interface diagram

No.	Name	Fuction
1	DC12V	Power interface
2	Switch	Control camera power
3	Indicator light	Indicate the camera status, press F2 to control the light on or off of the indicator light Red: Camera powered on Orange *: Normal operation
4	CameraLink interface	Camera data transfer
5	USB 3.0 interface	Camera data transfer
6-8	TRIG.OUT	External trigger output port, 6-8 corresponds to TRIG OUT 1-3, the default output signal is as follows: TRIG OUT1: Readout end signal TRIG OUT2: Global exposure signal TRIG OUT3: Exposure start signal The above trigger output signal types support customer customization settings
9	TRIG.IN	External trigger input interface (SMA interface)
10-11	Water cooling pipe joint	water cooling

*** Note:**

If the software has been shut down but the camera light remains orange, it indicates that the camera has not been fully released and needs to be completely exited from the camera thread or be restarted before the indicator light will return to red.

3. Features and Functions

3.1. Camera Introduction

The Dhyana 400BSI V3 is a new generation sCMOS camera with a 6.5-micron pixel size that perfectly matches high numerical aperture microscopes, balancing the demands for high spatial sampling rates and high sensitivity, adaptable to various application scenarios. This camera supports USB and CameraLink interface. Under CameraLink connection, the maximum readout speed of 100 frames per second at full resolution can be achieved. Additionally, to meet the needs of systems like Lightsheet, the Dhyana 400BSI V3 camera has developed a rolling shutter control mode. In this mode, users can customize parameters such as row exposure interval and scanning direction of the rolling shutter to achieve high signal-to-noise ratio synchronous imaging.

3.2. Structure and Operation of sCMOS

Scientific grade complimentary metal-oxide semiconductor (sCMOS) cameras are specialized cameras used for scientific research and high-performance imaging. They combine the advantages of CMOS and Charge coupled device (CCD) technologies, featuring high speed, low noise, and high sensitivity, and are widely used in scientific research, biomedical imaging, optical microscopy, and other fields.

The structure of an sCMOS camera sensor typically includes the following components:

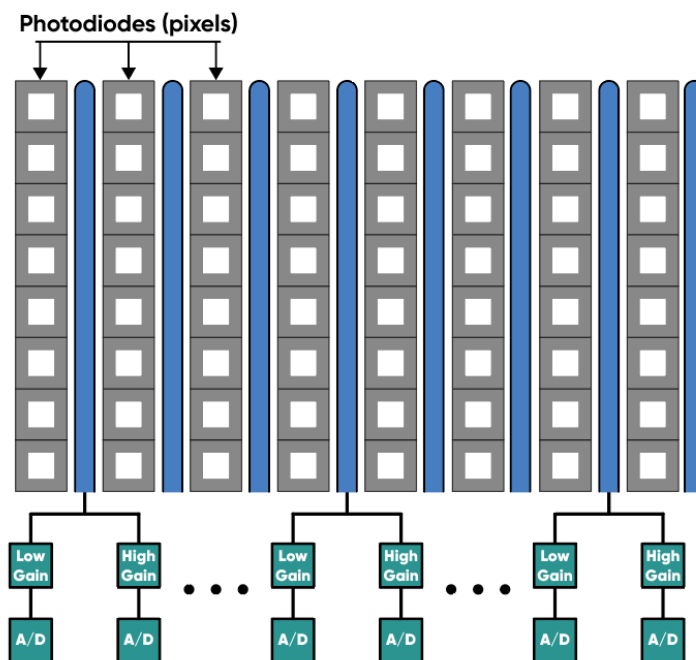


Figure 3-1 sCMOS camera sensor structure

- 1) Light-sensitive sensor array: sCMOS cameras use sCMOS sensor arrays (also known as image sensors) to capture light signals. These sensors consist of many photosensitive units that convert light into charge signals.
- 2) Gain amplifier: Each photosensitive unit in an sCMOS camera is equipped with an independent gain amplifier to amplify the charge signal and convert it into a voltage signal.
- 3) Analog-to-digital converter (ADC): The amplified analog signal is digitized through an analog-to-digital converter (ADC) inside the camera, converting it into a digital signal for further processing and storage.

sCMOS cameras typically also include an image processing unit for performing image enhancement, correction, and other image processing algorithms. The digitized image undergoes these processes to obtain higher-quality images.

The operation process of an sCMOS camera is as follows:

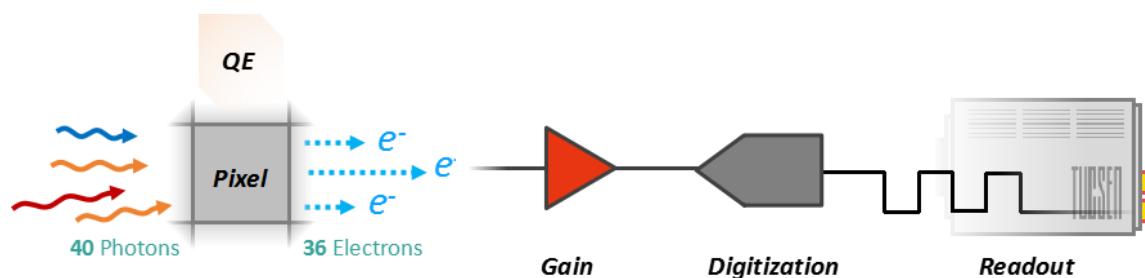


Figure 3-2 sCMOS operation process

- 1) Light signal capture: When photosensitive units are exposed to light, the light is converted into charge signals and stored in each unit.
- 2) Signal amplification: The charge signals from each photosensitive unit are amplified by corresponding gain amplifiers and converted into voltage signals.
- 3) Digitization: The amplified analog signals are converted into digital signals by an ADC for processing and storage.
- 4) Image processing: The digital signals undergo various algorithmic processes such as denoising, enhancement, and color correction through the image processing unit.
- 5) Data output: Processed image data can be transmitted to computers or other devices for display, analysis, and storage through various interfaces such as USB, Ethernet, etc.

3.3. Shutter Mode

The 400BSI V3 camera uses a rolling shutter readout mode. In this mode, the camera reads out

rows sequentially, with consistent exposure time for each row, but different starting exposure time point for different rows. The difference in exposure time points between adjacent rows is also known as the line time (T_{line}).

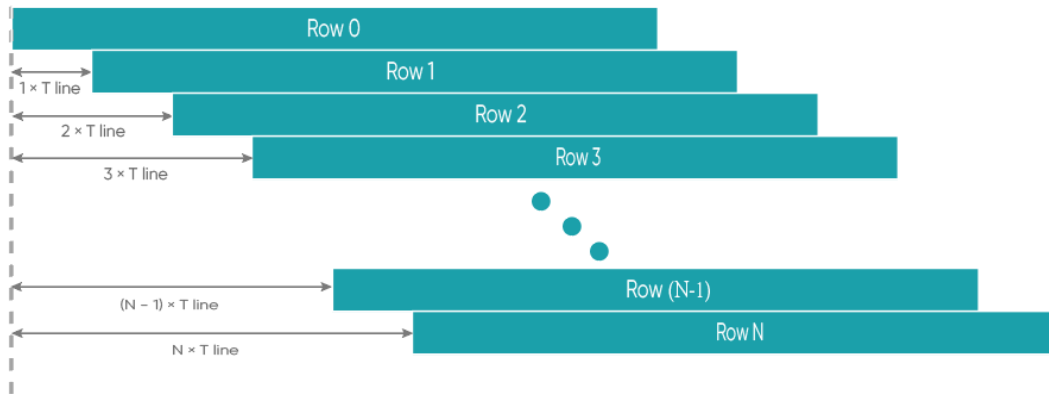


Figure 3-3 Rolling shutter diagram

In rolling shutter mode, if the camera is not synchronized with external light sources or if flickering light sources are present, it may result in striped images. This effect is especially noticeable with short exposure times (Please refer to the FAQs for solutions).

3.4. Front-Illuminated and Back-Illuminated sCMOS Technology

Cameras based upon sCMOS technology typically use two types of chips: front-illuminated (FSI) and back-illuminated (BSI). In front-illuminated cameras, light entering the pixels must pass through metal circuit structures before being detected. Due to the non-transparency of metal circuit structures, early cameras had only about 30-40% quantum efficiency (QE). Later, with the introduction of microlenses, light was focused through the conductors onto the photosensitive silicon, increasing QE to around 70%. Some advanced front-illuminated cameras can even achieve a peak QE of around 84%.

Back-illuminated cameras reverse this sensor design by placing the metal circuitry behind the photosensitive silicon layer, allowing incident photons to directly strike the thin photosensitive silicon layer. This process innovation significantly increases the peak QE of back-illuminated cameras and improves imaging quality in low-light environments. Due to the thin photosensitive silicon layer of back-illuminated pixels, there are higher process requirements and production difficulties compared to front-illuminated ones.

The 400BSI V3 camera adopts a back-illuminated chip, achieving a peak QE of around 95%.

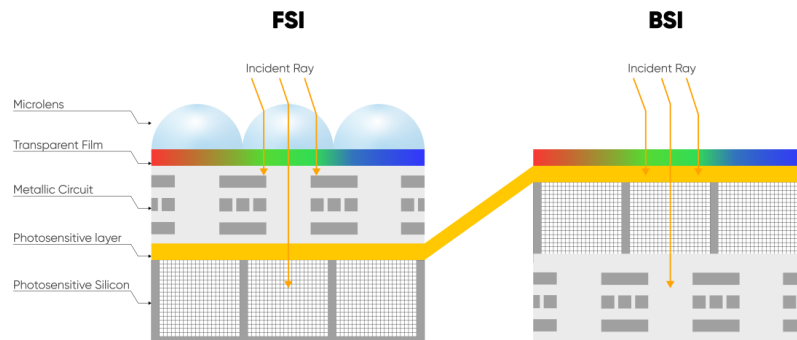


Figure 3-4 Front-Illuminated and Back-Illuminated diagram

3.5. Readout Noise

Readout noise is the noise introduced by the readout of the signal through the circuit. In CCD camera, since the readout circuit is the same for all pixels, the standard deviation (σ) for each pixel is generally consistent. Therefore, in CCD camera parameter tables, a single value—the root mean square (RMS) of the standard deviation of all pixels—can represent the readout noise.

However, each pixel in sCMOS corresponds to a different readout circuit, forming a distribution curve, shown in Figure 3-5. To illustrate the characteristics of this curve, sCMOS camera parameter tables typically provide two values—median and RMS. The median is the median of the standard deviations of all pixels, while the RMS is the root mean square of the standard deviations of all pixels. Since there are usually a few pixels with exceptionally high readout noise on the sCMOS camera chip—having less impact on the median than on the RMS—median values are generally lower than RMS values.

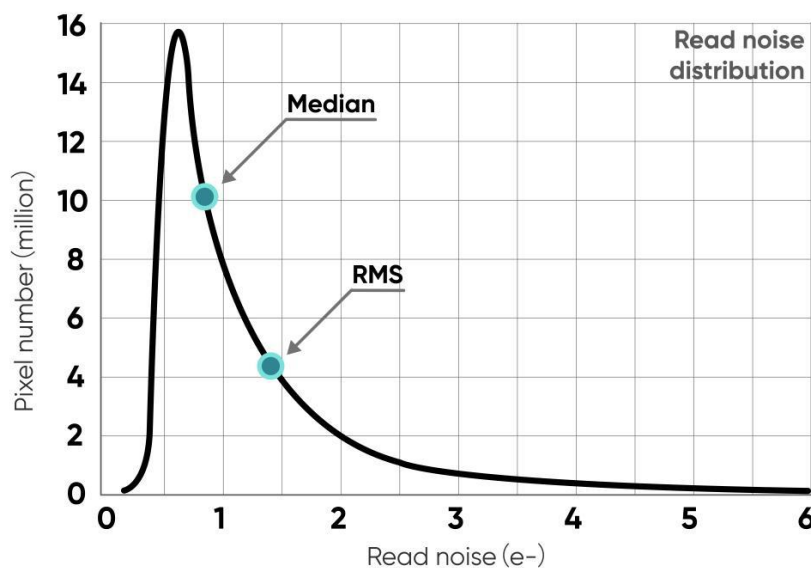


Figure 3-5 Readout noise distribution of an typical sCMOS camera

To measure and calculate readout noise from images, it's necessary to eliminate or minimize the influence of thermal noise and photon shot noise, retaining only the readout noise generated during the circuit readout process. Therefore, when measuring readout noise, it's typically done in an environment without light signals, with the exposure time set to the minimum value (to minimize the accumulation of dark current) to obtain dark-field images (called dark images). By capturing N such images, each pixel obtains N readout values—their standard deviation (σ) reflects the value of the readout noise for the corresponding pixel.

3.6. Defective Pixel Correction (DPC)

There are always a few abnormal values on the sCMOS camera chip. Through the camera's Defective Pixel Correction (DPC) function, these abnormal points can be corrected, removing defective pixels from the image. However, this may cause flickering pixels in some single-molecule imaging applications. It is not recommended to use the DPC function for these applications or to use only the weakest correction level.

The Dhyana 400BSI V3 adopts dynamic defective pixel correction, correcting using a 3x3 matrix of pixels. Currently, four correction levels are available, each corresponding to different thresholds, thereby controlling the intensity of defective pixel correction.

3.7. Dark Signal Non-Uniformity (DSNU)

When the camera captures images in complete darkness, ideally, all pixel grayscale values should be close to zero and equal. However, in reality, when the camera captures images in darkness, subtle differences in the performance of each pixel in the sensor will cause some variations in the pixel grayscale values outputted from the camera.

In practical applications, when there are no photons incident on the camera, the obtained image usually does not show a grayscale value of 0 (DN). This is because manufacturers typically set a offset value, such as 100 grayscale values, to account for the influence of noise on measurements based on this baseline in the absence of light. However, without careful calibration and correction, this fixed offset may also vary between different pixels. This variation is called "fixed pattern noise" and can be measured by DSNU (Dark Signal Non-Uniformity). It represents the standard deviation of pixel bias, measured in charge units.

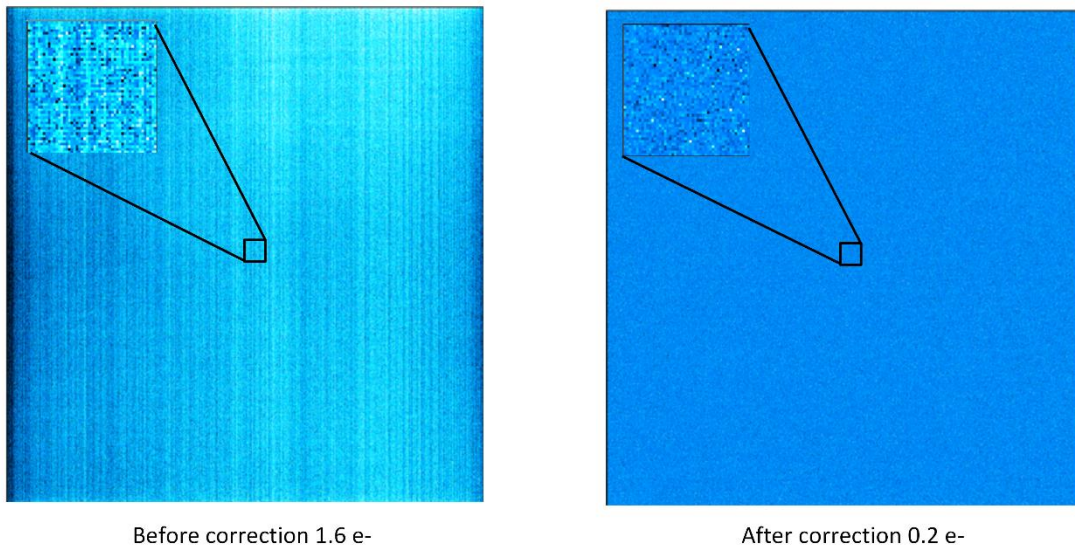


Figure 3-6 DSNU correction comparison before(left) and after(right)

For many low-light imaging cameras, DSNU is typically less than 0.5 e-. This means that in medium or high light level applications (where each pixel can typically capture hundreds or thousands of photons), the influence of this noise can be completely negligible. Moreover, even for low-light applications, if DSNU is lower than the camera's readout noise (typically 1-3 e-), this fixed pattern noise is unlikely to affect image quality.

3.8. Photo Response Non-Uniformity (PRNU)

When a camera captures uniformly illuminated light targets under bright light conditions, ideally, all pixel grayscale values should be close to the maximum grayscale value and equal. However, in reality, there are subtle differences in the performance of camera pixels, causing changes in pixel grayscale values outputted from the camera due to variations in lenses or illumination.

When the camera detects light signals, the number of photoelectrons captured by each pixel during the exposure process is measured and transmitted as digital grayscale values (DN) to the computer. The conversion from electrons to DN follows a certain proportion, called the system gain (K) or conversion gain, plus a fixed offset (usually 100 DN). These values are determined by both the analog-to-digital converters and amplifiers used for conversion. sCMOS cameras use parallel transmission, with one or more analog-to-digital converters per column of the camera and one amplifier per pixel, resulting in slight variations in pixel gain and offset.

Under dark field or low light conditions, differences in offset can be measured by DSNU as mentioned in Section 3.7. In bright environments, the influence of gain also needs to be considered. Differences in gain and offset changes are measured by Photo Response Non-Uniformity (PRNU), which is the ratio of detected electrons to displayed DN. Given that the

intensity values produced will vary depending on the signal size, PRNU is expressed as a percentage.

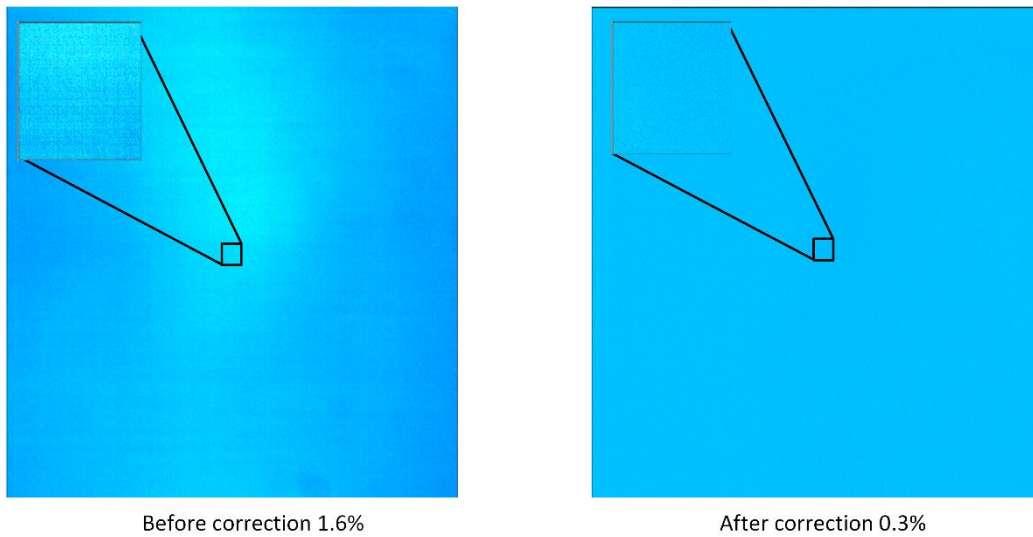


Figure 3-7 PRNU correction comparison before(left) and after(right)

Typical PRNU values are < 1%. For all low-light and medium-intensity light source imaging (signals of 1000 e- or less), this variation is negligible compared to readout noise and other sources of noise. Similarly, when imaging at high light levels, this variation is not significant compared to other noise sources in the image (such as photon shot noise). However, in high light level imaging applications requiring very high measurement accuracy, especially those using frame averaging or frame summation, PRNU values < 1% are highly necessary.

3.9. Gain Mode

The 400BSI V3 camera has four gain modes: High Dynamic Range (HDR) mode, High Sensitivity mode, High Speed mode, and Global Reset mode. Each mode has differences in synthesis principles, line times, gain values, and readout noise. Selecting the appropriate mode based on the actual scenario is essential to obtain high-quality imaging results.

Table 3-1 Typical gain mode parameter table*

Mode	HDR (16bit)	High Sensitivity (12bit)	High Speed (11bit)
System gain (DN/e-)	1.4	2.3	0.9
Full-Well Capacity (e-)	45000	1500	2000
Readout noise(e-)	1.6(Median)	1.1(Median)	1.9(Median)
	1.7(RMS)	1.2(RMS)	2.0(RMS)

***Note:**

The values in this table are typical and may vary between different cameras. Please refer to the factory photoelectric report for specific details.

3.9.1. High Dynamic Range

High Dynamic Range (HDR) mode synthesizes images with different analog gains but the same exposure time. It includes Low Gain (LG) mode with high full well capacity and high noise suitable for imaging strong signals, and High Gain (HG) mode with low full well capacity and low readout noise suitable for imaging weaker signals. Combining high and low gain images through algorithms generates an HDR image. This mode is suitable for applications with large variations in signal strength.

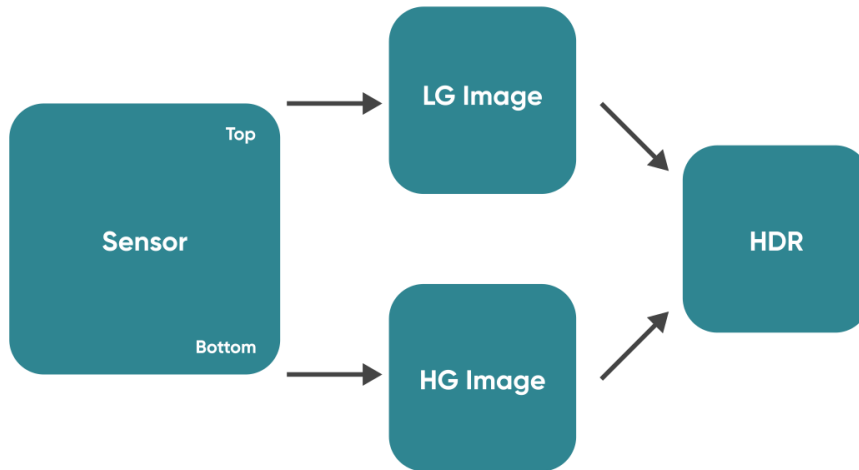


Figure 3-8 Schematic diagram of HDR mode

3.9.2. High Sensitivity

High Sensitivity mode utilizes Correlated Multiple Sampling (CMS) technology, also known as the CMS mode, typically with 2x sampling, to reduce noise by $\sqrt{2}$ times. Each row's data is collected from both top and bottom channels simultaneously and then averaged after overlaying both images to generate a CMS mode image. This mode is configured with higher gain and is suitable for applications with weak signals.

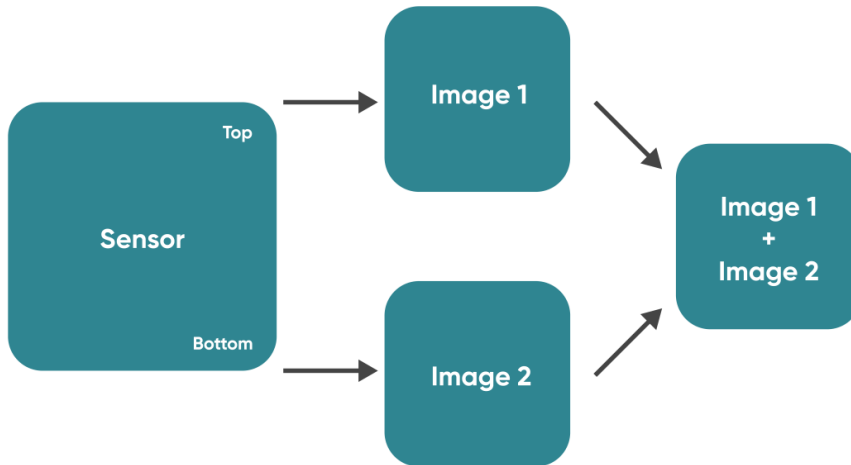


Figure 3-9 Schematic diagram of High Sensitivity mode

3.9.3. High Speed

High Speed mode simultaneously outputs odd and even rows from both top and bottom readout chains to increase the frame rate. This mode is typically suitable for applications requiring a certain frame rate, such as dynamic observation.

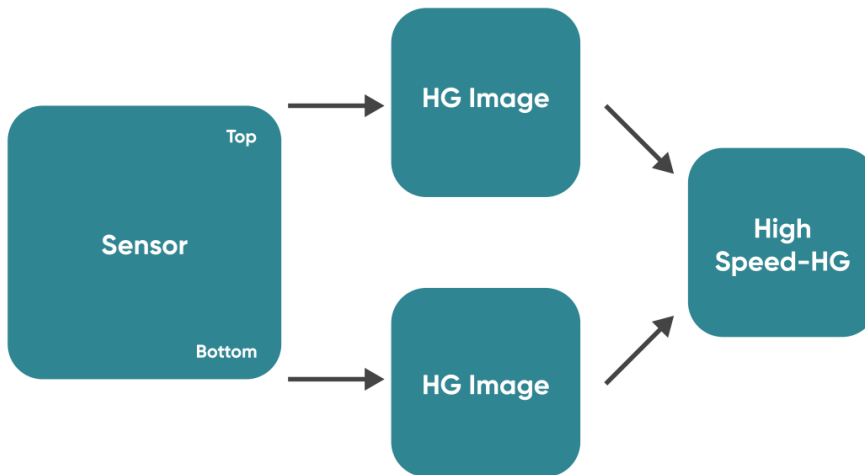


Figure 3-10 Schematic diagram of High Speed mode

3.9.4. Global Reset

Global Reset mode enables the camera to achieve the shooting effect of a global shutter camera. It first resets the entire pixel array of the chip simultaneously, then exposes all rows simultaneously. After exposure, data is read out row by row, with the exposure time increasing row by row. In ideal applications, the light source should be turned off immediately after the

exposure of the first row to avoid obtaining unevenly illuminated images. This mode is suitable for applications requiring synchronized signals and can be used to capture transient objects.

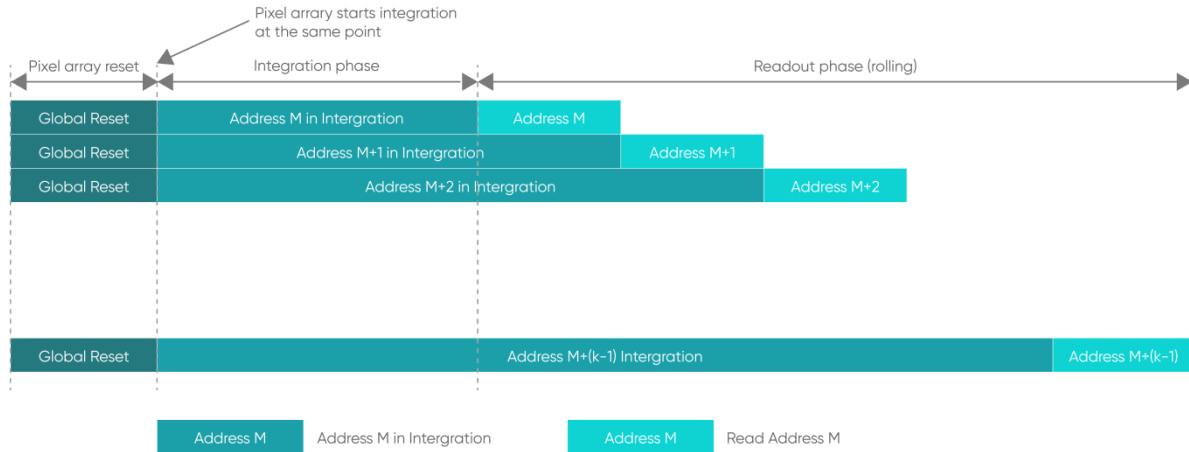


Figure 3-11 Global Reset mode diagram

3.10. Region of Interest Readout

In imaging applications, ROI (Region of Interest) defines a subregion of interest within the camera sensor's resolution range, and selecting an ROI allows only the images within this subregion to be read out. Rolling shutter cameras can increase the camera's readout speed by reducing the number of rows. The software sets preset subregions and also supports manual settings, where the row window must be a multiple of 4, and the column window must be a multiple of 8.

Typical ROI frame rates for different interfaces of the camera can be found in Table 3-2, Table 3-3:

Table 3-2 Typical ROI area measured frame rate (fps) table for Dhyana 400BSI V3 camera under USB 3.0

Column (Pixel)	Row (Pixel)	HDR	High Sensitivity	High Speed	Global Reset
2048	2048	43	43	60	43
2048	1024	86	86	121	86
2048	512	173	173	241	173
2048	256	344	344	484	344
2048	128	681	681	965	672
2048	64	1331	1331	1916	1314
2048	8	8072	8072	9152	7461

Table 3-3 Typical ROI area measured frame rate (fps) table for hyana 400BSI V3.0 camera under CameraLink

Column (Pixel)	Row (Pixel)	HDR	High Sensitivity	High Speed	Global Reset
2048	2048	43	43	100	43
2048	1024	86	86	200	86
2048	512	172	172	397	172
2048	256	342	342	792	342
2048	128	678	678	1578	678
2048	64	1327	1327	3135	1305
2048	8	8113	8113	19841	7432

Note:

- 1) The minimum supported ROI for Dhyana 400BSI V3 on Mosaic V3 is 48 (columns) × 8 (rows).
- 2) Frame rates are affected by computer system configuration, and it is recommended to use a computer with an i5 processor or above and a 64-bit system.
- 3) For high-speed image acquisition, it is recommended to uncheck automatic levels and turn off the Image Adjustment module.
- 4) The frame rates in the above table are the measured maximum values under the shortest exposure time.

3.11. Binning Readout

Binning is a readout mode that recombines camera pixels, which can improve sensitivity but may also reduce resolution. For example, 2 x 2 binning combines every 4 pixels (2 rows 2 columns) into one "large pixel", and the camera outputs one pixel intensity value.

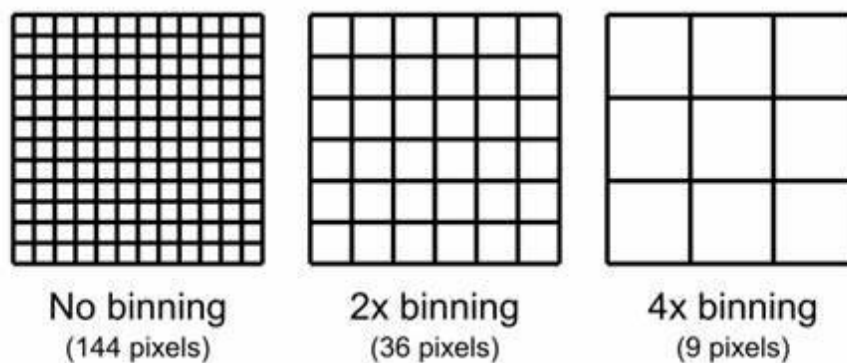


Figure 3-12 Schematic diagram of Binning

Binning can be performed by the camera's FPGA or by the camera operating software. Combining signals in this way can improve the signal-to-noise ratio, enabling the detection of weaker signals, improving image quality, or shortening exposure times. However, the effective pixel size of the camera also increases, which may reduce the camera's resolution of target details.

Binning data processing can be divided into Sum Binning and Average Binning. In 2 x 2 Binning, for example, Sum Binning adds the grayscale values of four pixels, while Average Binning adds the grayscale values of four pixels and then divides by 4 to obtain the average grayscale value.

The software Binning selection on Mosaic V3 is shown below:

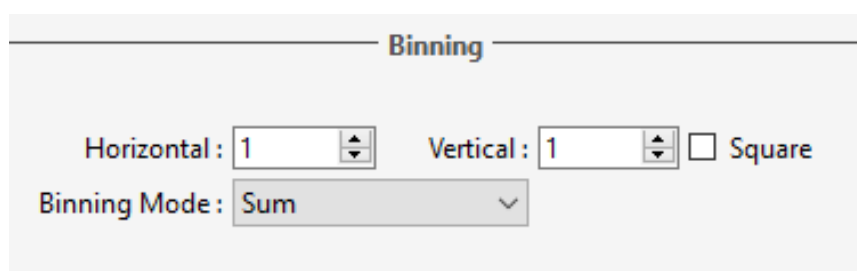


Figure 3-13

The FPGA Binning selection on Mosaic V3 is shown below:

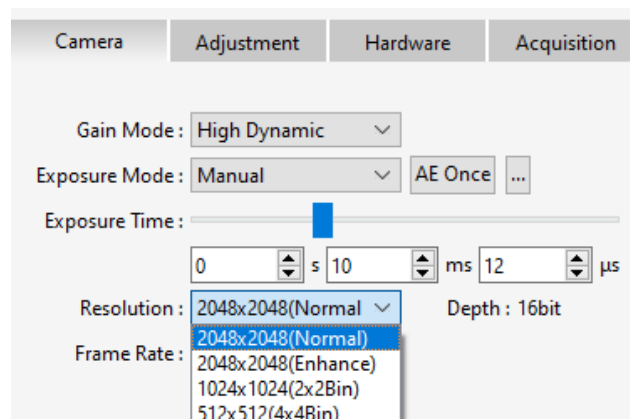


Figure 3-14

The 2048 x 2048 (Enhance) resolution uses Tucsen's own signal enhancement algorithm, which differs from 2 x 2 Binning in that it accumulates neighboring four pixels into one output pixel, effectively improving the signal-to-noise ratio without sacrificing resolution. It should be noted that using this algorithm will modify the original pixel value, which is not recommended for users who need to quantify.

3.12. Timestamp

The camera accurately reads the start time of each frame with a time precision of 1 μ s. In Mosaic V3 software, images are saved in .sen format, and timestamp information is displayed in the image information, supporting the export of image information to .csv format files.

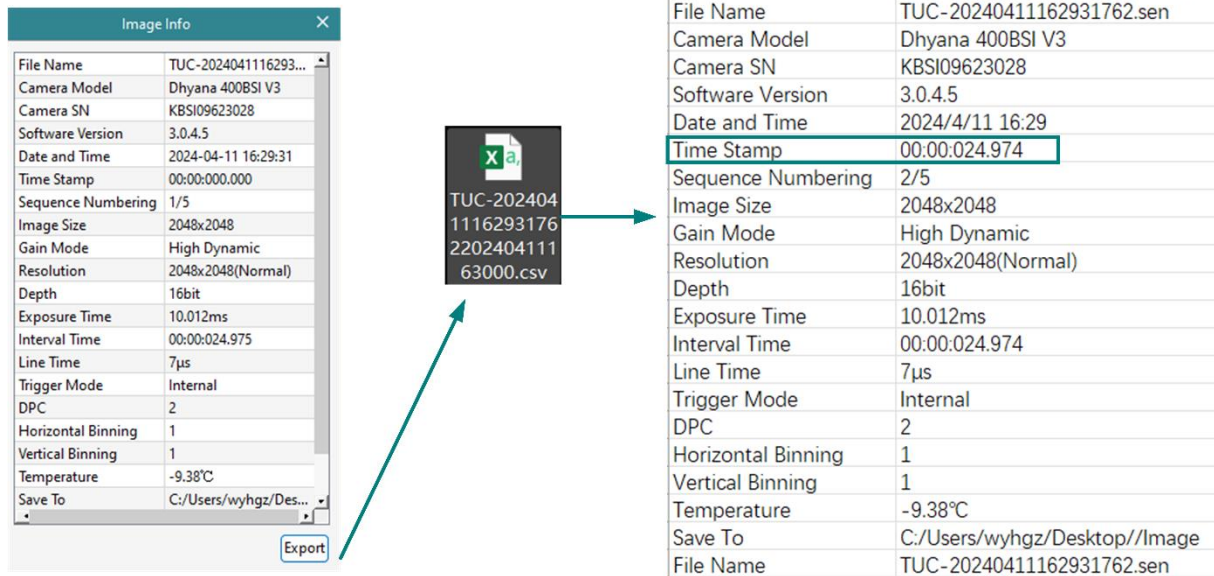


Figure 3-15 Timestamp export schematic

Note:

Applications requiring timestamp functionality generally have high time precision requirements, and it is recommended to use the To RAM image storage mode.

3.13. Frame Rate Calculation

The camera's frame rate is affected by the readout time and the exposure time. The theoretical frame rates can be calculated using the formulas provided in Tables 3-5 and 3-6.

The line time and theoretical full-width minimum readout time for each mode of the Dhyana 400BSI V3 are shown in the following table.

Table 3-4 Calculation of readout time

Gain mode	Line time (T_{line})	Readout Time ($T_{readout}$)
High Dynamic Range High Sensitivity Global Reset	11.2 μ s	2048*11.2 μ s=22.9376 ms
High Speed	7.2 μ s	2048/2*7.2 μ s=7.3728 ms

Typical frame rate calculations for CameraLink

Where H_n : The number of rows selected horizontally; V_n : The number of rows selected vertically; T_{line} : Line time; T_{exp} : The set exposure time; Y_{CL} : 100 fps (Maximum frame rate at full frame in CameraLink)

Table 3-5 Calculation of frame rate for CameraLink

Gain mode	Line time T_{line}	Calculation formula	Horizontal (H_n)	Vertical (V_n)	Frame rate (fps)
High Dynamic Range High Sensitivity	11.2 μ s	$1/\{(V_n+3)*T_{line}\}$	2048	2048	43.5
				1024	86.9
				512	173.4
				256	344.7
				128	681.6
				64	1332.6
Global Reset	11.2 μ s	$1/\{(V_n+4)*T_{line}+T_{exp}\}$	2048	8	8116.9
				2048	43.5
				1024	86.9
				512	173.0
				256	343.4
				128	676.4
High Speed	7.2 μ s	$1/(V_n/2048/Y_{CL})$	2048	64	1313.0
				8	7440.5
				2048	100.0
				1024	200.0
				512	400.0
				256	800.0
128	1600.0				
64	3200.0				
8	25600.0				

Typical frame rate calculations for USB 3.0

Where H_n : The number of rows selected horizontally; V_n : The number of rows selected vertically; T_{line} : Line time; T_{exp} : The set exposure time; Y_{U3} : 60 fps (Maximum frame rate at full frame in USB 3.0)

Table 3-6 Calculation of frame rate for USB 3.0

Gain mode	Line time T_{line}	Calculation formula	Horizontal (H_n)	Vertical (V_n)	frame rate (fps)
High Dynamic Range High Sensitivity	11.2 μ s	$1/\{(V_n+3)*T_{line}\}$	2048	2048	43.5
				1024	86.9
				512	173.4
				256	344.7
				128	681.6
				64	1332.6
				8	8116.9
Global Reset	11.2 μ s	$1/\{(V_n+4)*T_{line}+T_{exp}\}$	2048	2048	43.5
				1024	86.9
				512	173.0
				256	343.4
				128	676.4
				64	1313.0
				8	7440.5
High Speed	7.2 μ s	$1/(V_n/2048/Y_{U3})$	2048	2048	60.0
				1024	120.0
				512	240.0
				256	480.0
				128	960.0
				64	1920.0
				8	15360.0

Note:

- 1) The frame rate is affected by the actual transmission bandwidth and computer system configuration, and to prevent frame loss, the actual transmission will increase the interval time in units of line time, and the readout time will increase accordingly, resulting in part of the calculated frame rate may be greater than the actual frame rate;
- 2) Frame rate table values are calculated at the lowest exposure time, HDR/High Sensitivity/High Speed modes with $T_{exp} > T_{readout}$, frame rate = $1/T_{exp}$ (s);
- 3) The maximum bandwidth of USB3.0 is about 360MB/s, and the maximum bandwidth of CameraLink is about 800MB/s.

3.14. Frame Rate Adjustment

Each frame image readout has a fixed blanking time, and frame rate adjustment is achieved by changing the blanking time (T blanking) to control the frame rate.

For example, if the exposure time < readout time, considering a frame rate of 60 fps, setting the frame rate to 40 fps adds 8.33 ms of blanking time during image output.

Similarly, if the exposure time > readout time, considering an exposure time of 100 ms, setting the frame rate to 5 fps adds 100 ms of blanking time during image output.

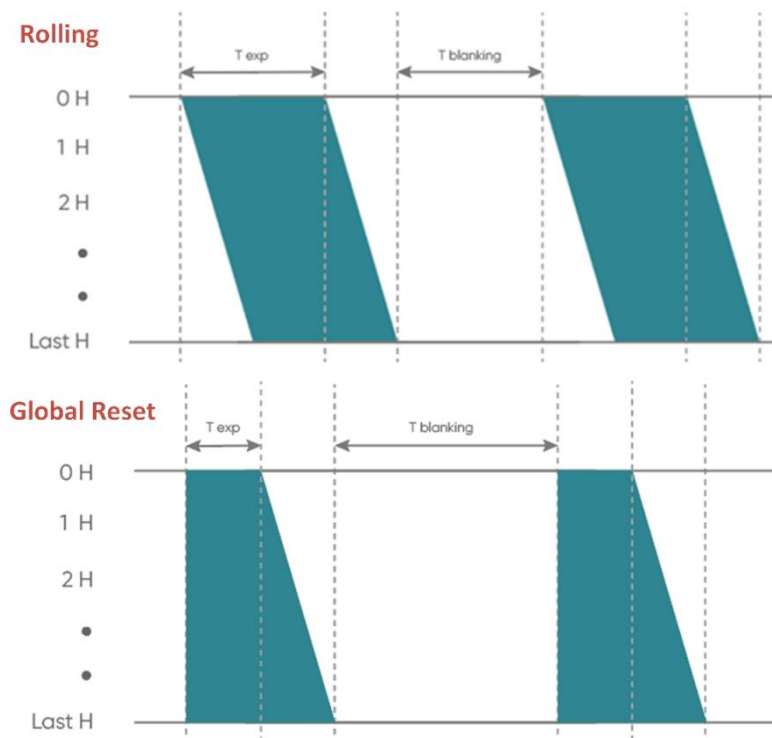


Figure 3-16 Frame rate adjustment timing diagram

3.15. Incident Photon Calculation

Scientific camera imaging involves the conversion of photons, electrons, voltage, and grayscale values. Therefore, it is possible to reverse calculate the incident number of photons from the grayscale values. The calculation formula is as follows:

$$P = \frac{(DN - Offset)/K}{Q(\lambda)}$$

Where: P represents the incident number of photons. DN is the grayscale value of the light signal. K is the system gain (refer to Table 3-1) in (DN/e⁻). Q(λ) corresponds to the quantum efficiency at the wavelength. Offset is the camera's background value in DN.

3.16. Acquisition Mode

3.16.1. Live mode

Live mode is suitable for real-time preview, providing data stream output. Images are continuously output like a flowing stream. In this mode, users can freely modify settings such as exposure time, gain mode, region of interest, etc., for real-time preview and image capture operations.

After successfully installing the Mosaic V3 software and drivers, the hardware trigger mode defaults to "internal trigger" (live mode), the user can click Preview/Stop to control the opening and closing of the camera live mode, and click Capture to obtain the image.

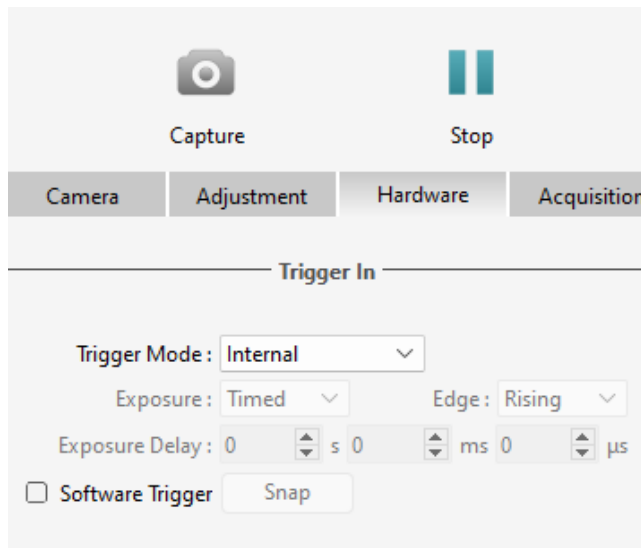


Figure 3-17

Users can set the exposure time, gain mode and other camera parameters, and preview them in real time through the preview window to get a suitable image.

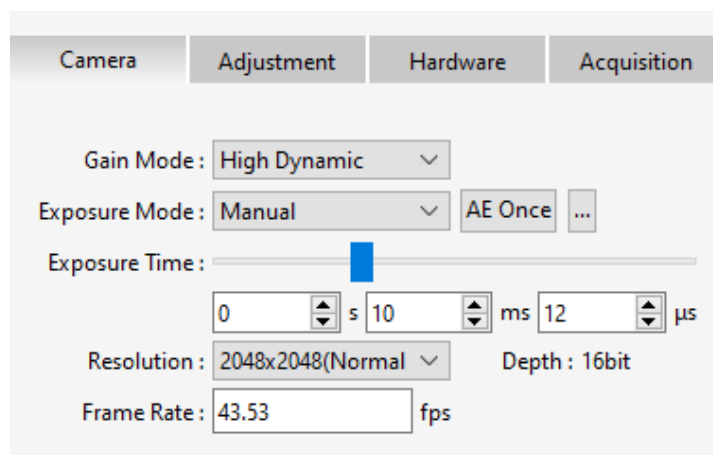


Figure 3-18

In the acquisition module, users can set the save path, file name, total number of frames and other information, and the image can be taken after the setting is completed.

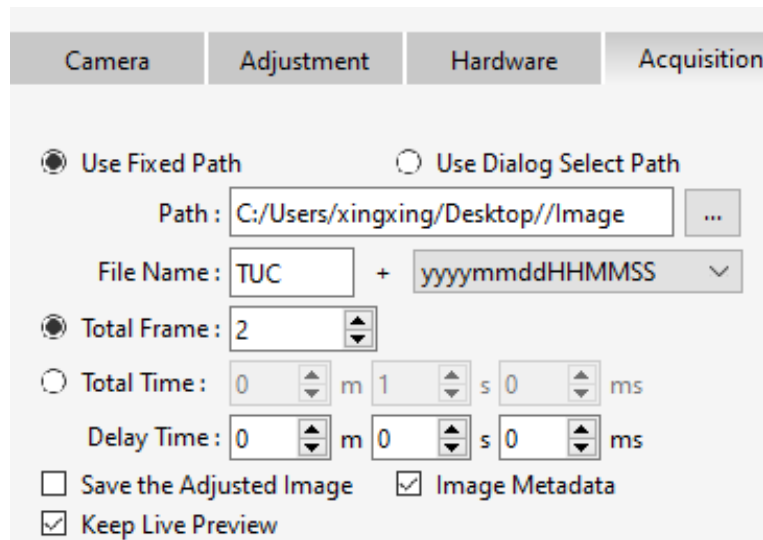


Figure 3-19

3.16.2. Software Trigger Mode

When the camera is in Software trigger mode, the software gives the camera a command to take a picture, and when the camera receives the signal, it starts the exposure and outputs the image. To use the software trigger mode in Mosaic V3, check the software trigger, click Capture to enter the waiting trigger state, and then click the **Snap** to execute the image capture command, and only output one image at a time.

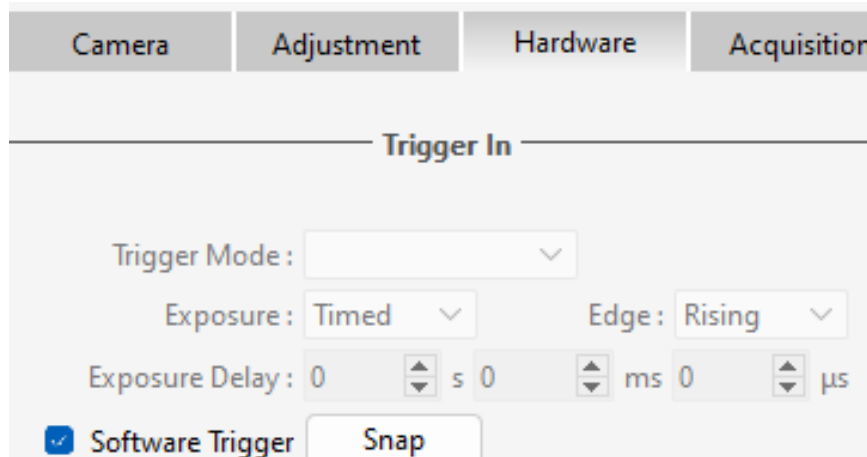


Figure 3-20

3.16.3. Hardware Trigger Mode

Hardware trigger mode waits for an external level trigger signal command to capture an image. It includes three modes: Standard Overlap, Standard Non-Overlap, and Synchronization.

The Mosaic V3 software provides configurations such as mode, frames/signal, exposure, edge, exposure delay, etc., to control the number of triggered images captured continuously according to the set quantity.

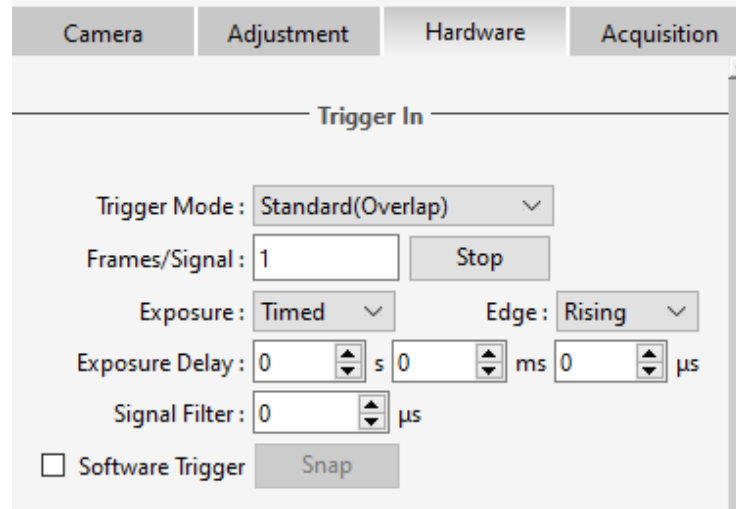


Figure 3-21

3.16.3.1. Hardware Trigger input circuit

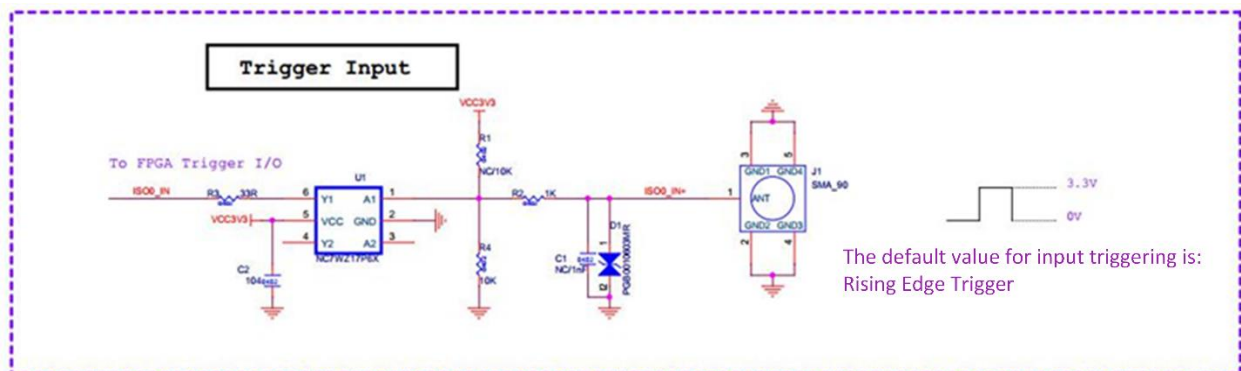


Figure 3-22 Hardware trigger input circuit

Note:

- 1) The valid external trigger signal recognized by the imager must be a level signal of 3.3 to 5 V. Exceeding the maximum voltage limit may cause permanent damage;
- 2) The pulse width of the recognized level signal must be greater than 1 μs.

3.16.3.2. Trigger Filtering

To suppress interference in the external trigger signal, external trigger filtering supports high and low-level filtering. This function filters out spikes in the level signal. The filtering time range can be set to [0, 1000000] μs, with the default being 0.

The following figure takes the filtering time set to 1 ms as an example:

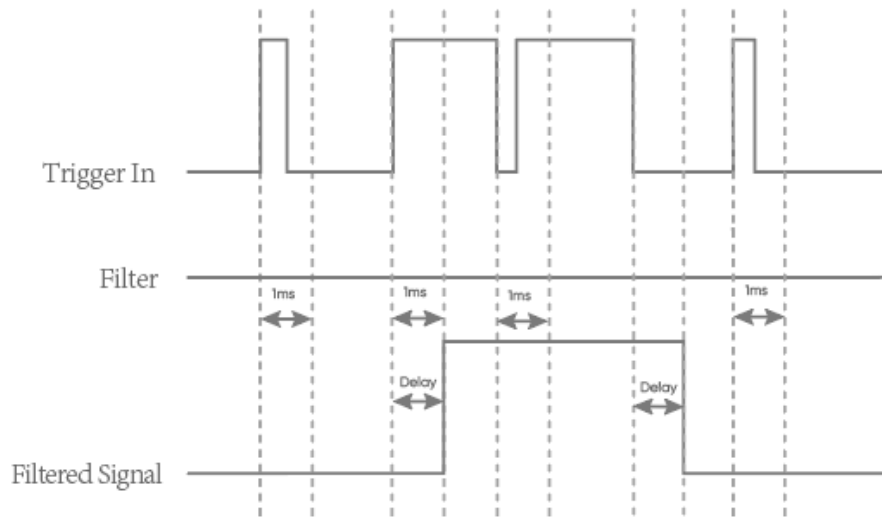


Figure 3-23 Trigger Filter function schematic

Note:

After the camera receives a valid trigger signal, the filter signal will lag behind the last edge of the jitter time period, with the lag time = the set filter time.

3.16.3.3. Trigger Delay and Jitter

The trigger delay and jitter for the HDR, High Sensitivity, and High Speed modes are shown below. When the external trigger signal arrives, there is a nanosecond-level delay T_{iso} through the hardware circuitry. After the delay through the hardware circuitry, the level signal input to the camera's internal undergoes conversion, resulting in some jitter T_{logic} , ranging from 0-1 minimum exposure unit T_{line} . Therefore, the total delay time from external trigger input to exposure start is $T_{delay} = T_{iso} + T_{logic}$, within the range of one line time. If the Trigger Filter function is used, a Trigger Filter Delay Time T_{filter} is added to this.

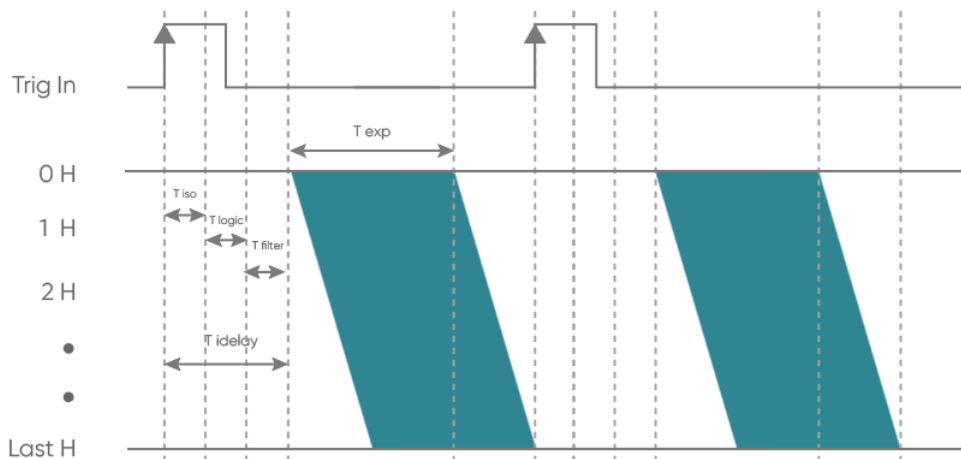


Figure 3-24 Schematic of trigger delay under Rolling

The delay and jitter in Global Reset mode is 600 ns, and if the trigger filter function is enabled, a trigger filter delay time T_{filter} will be added on top of this. the timing diagram is as follows:

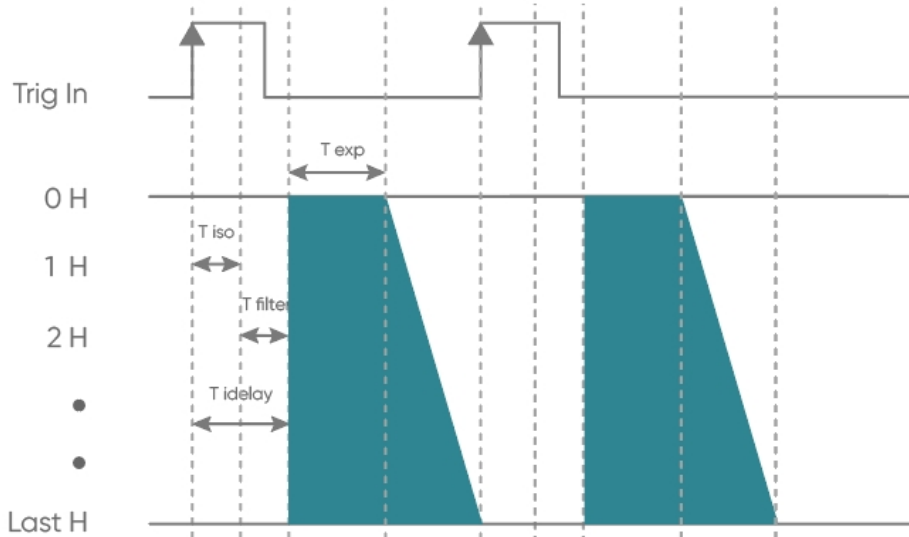


Figure 3-25 Schematic of trigger delay under Global Reset mode

T_{exp} : exposure time; T_{iso} : hardware circuit delay; T_{logic} : trigger jitter; T_{idelay} : total delay time; T_{filter} : trigger filter delay time; 1H: one T_{line}

3.16.3.4. Standard Trigger Mode

Standard trigger mode is divided into Standard (Overlap) trigger mode and Standard (Non-Overlap) trigger mode.

Standard (Overlap) Trigger Mode: In this mode, when the camera is in live mode, it responds to the trigger signal immediately after the first row of exposure ends.

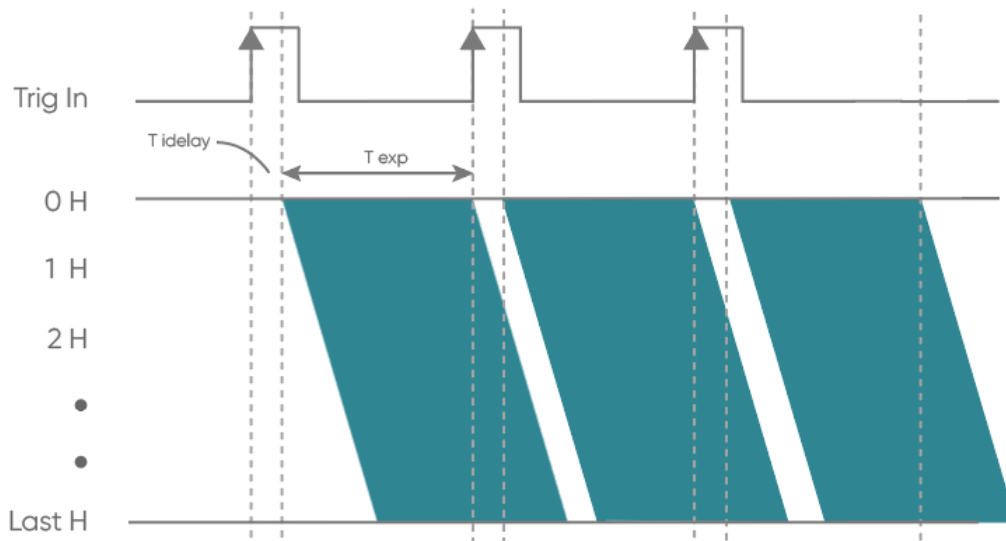


Figure 3-26 Standard (Overlap) Trigger timing

Standard (Non-Overlap) Trigger Mode: In this mode, when the camera is in live mode, it responds to the external trigger signal only after the readout ends.

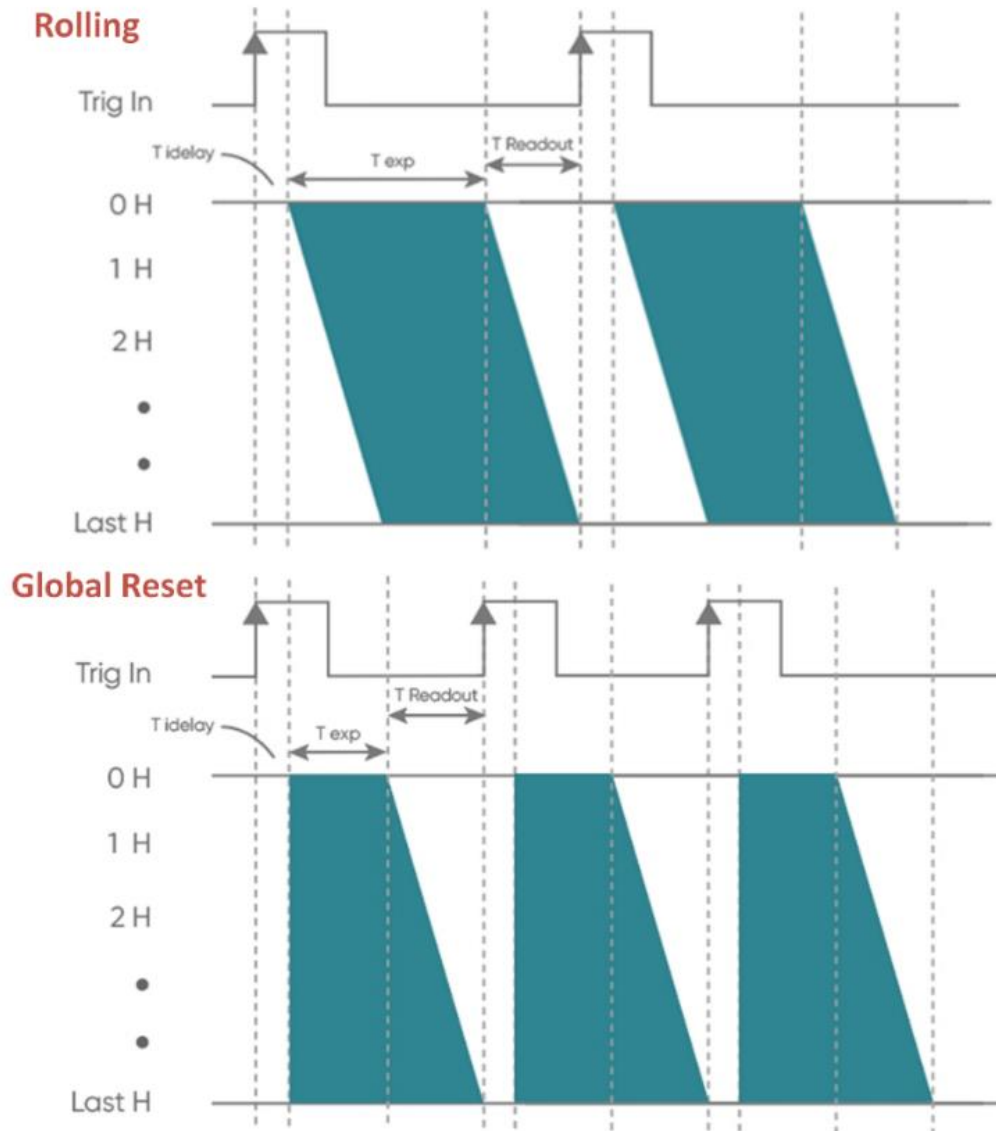


Figure 3-27 Standard (Non-Overlap) Trigger timing

Both of these modes support both level and edge triggering. In Standard (Non-Overlap) Trigger Mode, for example, in level trigger mode (i.e., the exposure type is selected as Width in the software), exposure start and end are controlled by the duration of the trigger signal's high or low level. Level trigger mode is not continuous shooting; it is commonly used to capture stationary or slowly moving objects.

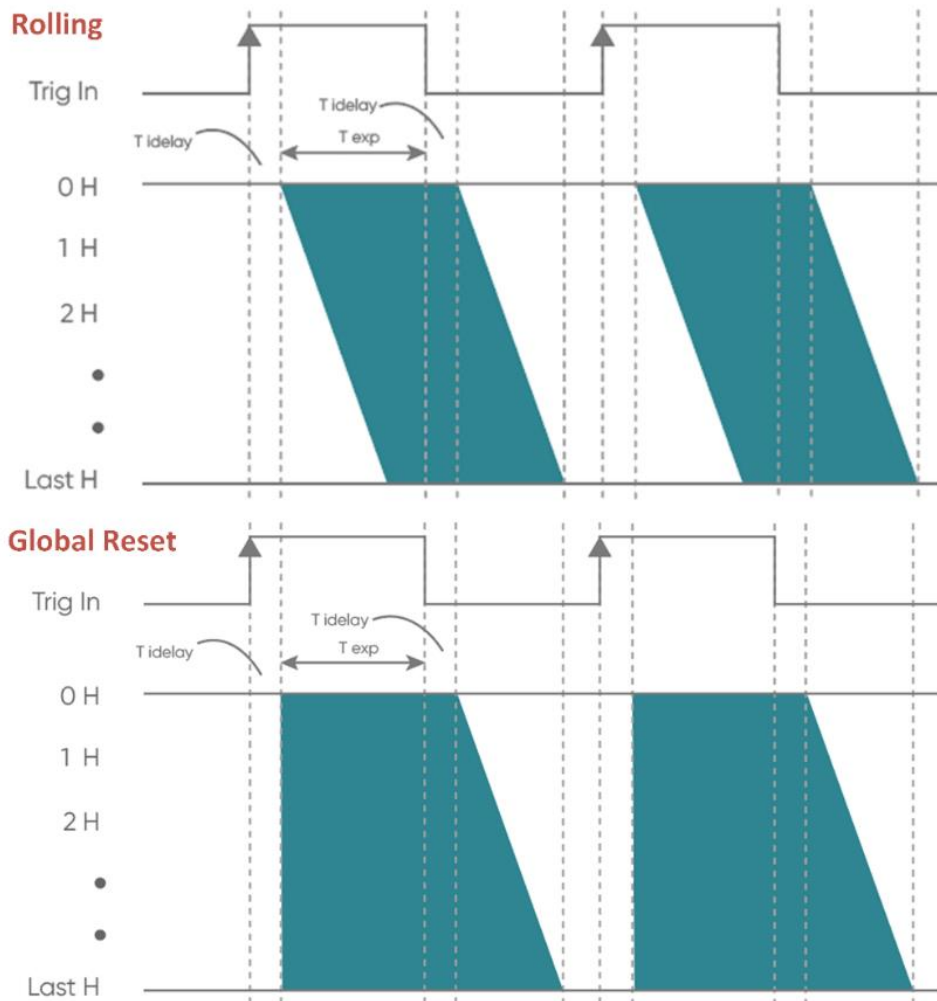


Figure 3-28 Non-Overlap Level Trigger timing diagram

Note:

Overlap triggering is not supported using Global Reset mode.

In the edge trigger mode (i.e., the exposure type is selected as Timed in the software), the length of the exposure time is set directly on the software interface. When using, it should be noted that the time of each pulse cycle of the trigger signal (pulse duration + pulse interval) must be greater than or equal to the total time used for each frame of image output (i.e., the reciprocal of the frame rate) to ensure that a frame of image is complete and error-free.

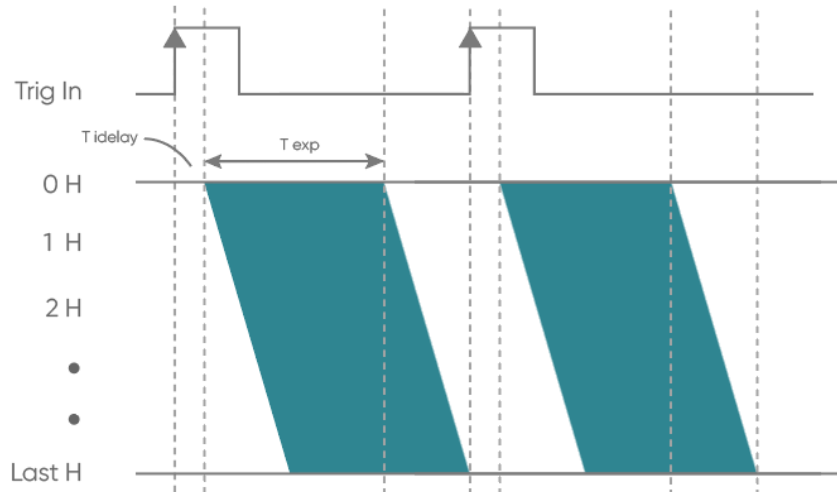


Figure 3-29 Edge Trigger timing diagram

400BSI V3 camera supports single-trigger multi-frame acquisition function, you can modify the number of triggering out of the picture by setting the frame/signal in the standard triggering mode (refer to Figure 3-21), for example, by setting the number of 2, the triggering timing diagram is as follows:

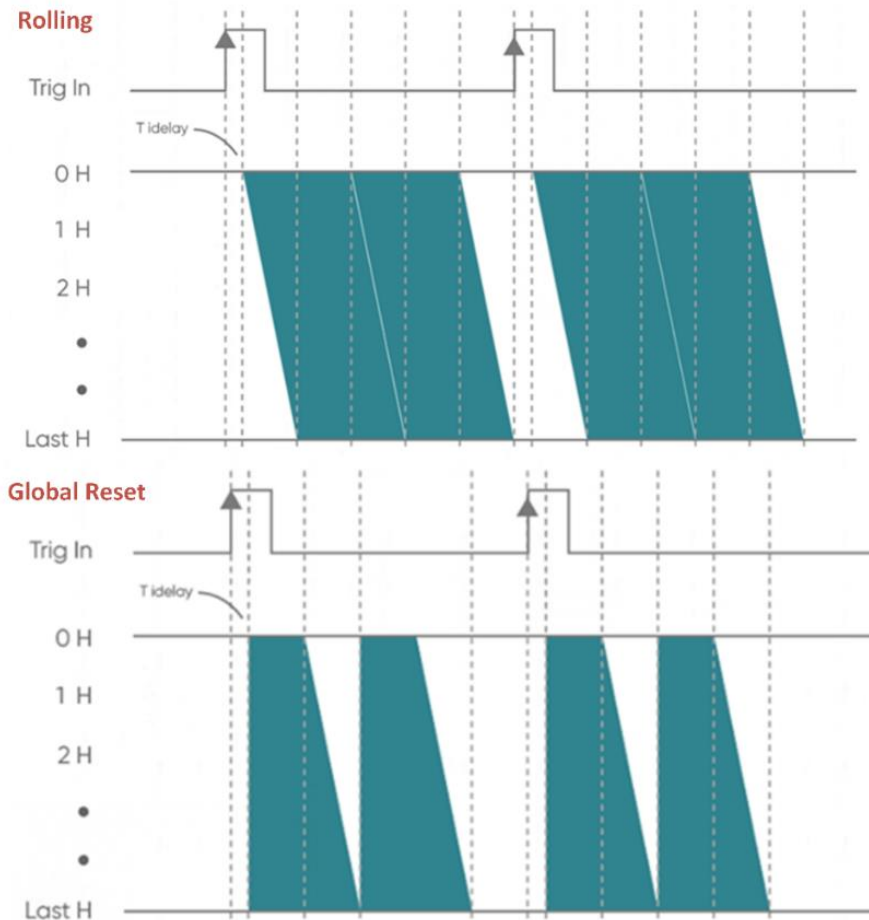


Figure 3-30 Single-trigger multi-frame acquisition timing diagram

3.16.3.5. Synchronization Trigger Mode

In this mode, when the camera receives a certain level signal, it starts exposure capture. When it receives the next level signal, it ends exposure, starts readout, and begins a new exposure cycle. This mode ensures complete synchronization of exposure start and readout with the external trigger signal.

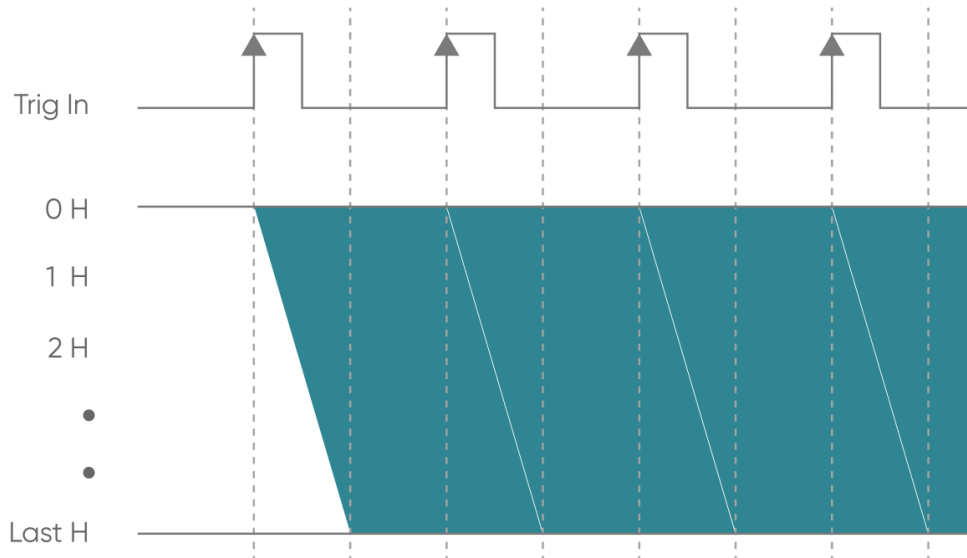


Figure 3-31 Synchronization Trigger mode timing diagram

The length of exposure time in this mode is determined by the time interval between the arrival of two trigger signal edges. After entering this mode, the camera starts the first frame exposure when the first trigger signal edge is detected, and does not terminate the first frame exposure and output the image until the trigger signal edge is detected for the second time, and at the same time starts the second frame exposure, and so on; that is, there is no image data for the first trigger signal after entering this mode, and there is an image output for each of the subsequent trigger signals, and the exposure time for each frame is the time interval between the arrival of the two trigger signal edges. The exposure time corresponding to each frame is the time interval between the arrival of the two trigger signal edges. The same mechanism is followed when the trigger signal is single pulse or multi-pulse.

This mode is very useful for confocal microscopy as it enables simultaneous control of the camera's exposure time and spinning disk confocal speed to eliminate the effects of inhomogeneous light.

3.16.4. Rolling Shutter Control Mode

Rolling shutter control is supported in Dhyana 400BSI V3 camera. This mode utilizes the characteristic of rolling shutter readout, allowing seamless synchronization with the movement of LightSheet imaging systems. This mode significantly improves the signal-to-noise ratio of

images by repeatedly exposing samples from top to bottom or bottom to top, line by line. It is mainly used in life sciences, especially in applications such as neural development microscopy.

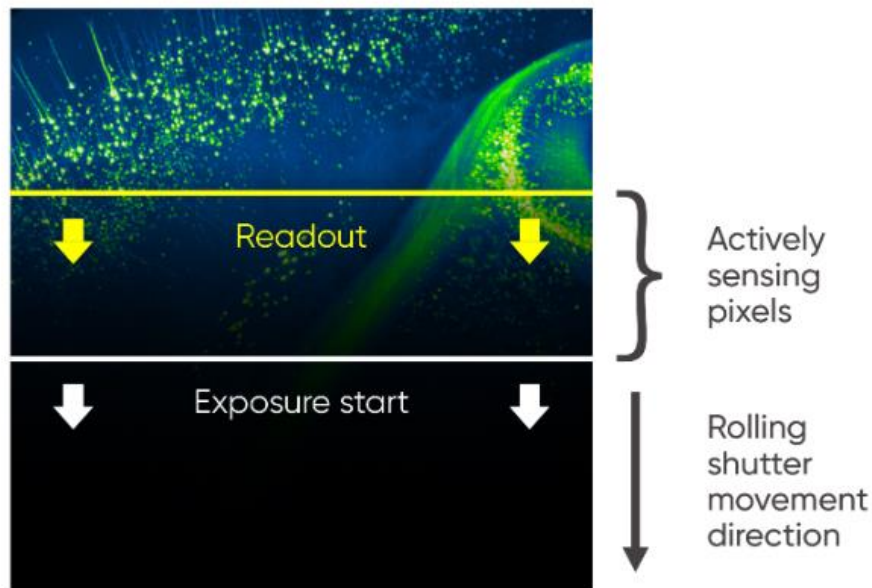


Figure 3-32 Schematic diagram of Rolling Shutter Control

The implementation of the rolling scan control mode requires firmware to operate the SENSOR imaging chip: adding a delay to the reset signal and the readout signal to control the time at which the exposure starts for each line after the first line, and to control the synchronization of the active exposure area and external illumination within a more flexible line time frame, thus enabling efficient and fast imaging.

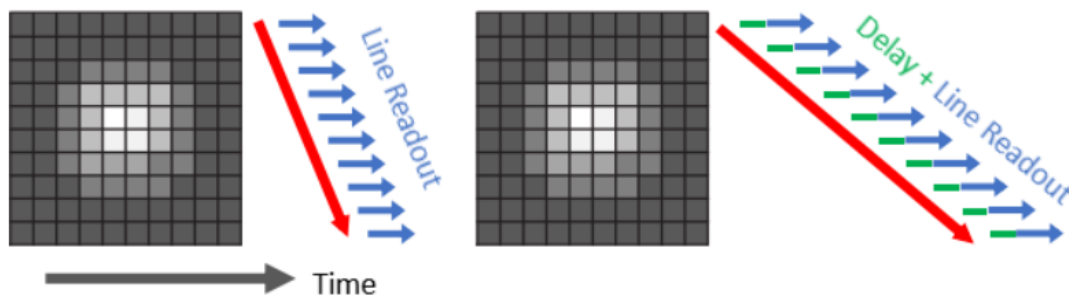


Figure 3-33 Schematic diagram of Rolling Shutter Control

LightSheet user can define the "line time delay" or "Slit Height" to enable the LightSheet system flexibly scanned simultaneously, and the scanning direction can be set from top to bottom or bottom to top to meet different application needs.

There are three options for the direction of the rolling shutter:

Down: The downward scanning direction is the default scanning direction for sCMOS cameras. The rolling shutter starts at the top of the sensor and scans down to the bottom of the last line. Each subsequent frame acquisition starts with the first line at the top.

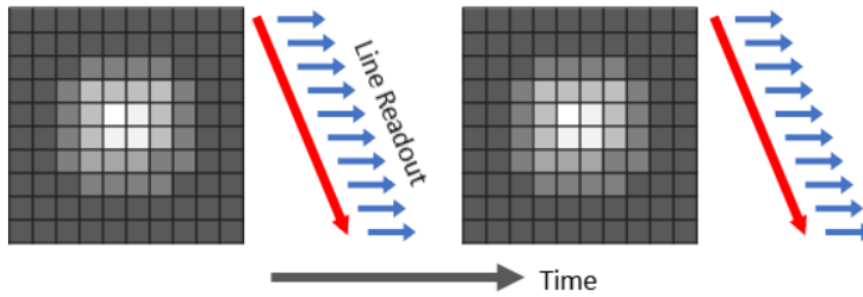


Figure 3-34 Schematic diagram of Down scanning

Up: Upward scanning mode, the rolling shutter scans upwards from the bottom line to the top first line. Each subsequent frame acquisition starts with the bottom line. The image orientation acquired in this mode is not reversed and is consistent with the image in scan down mode.

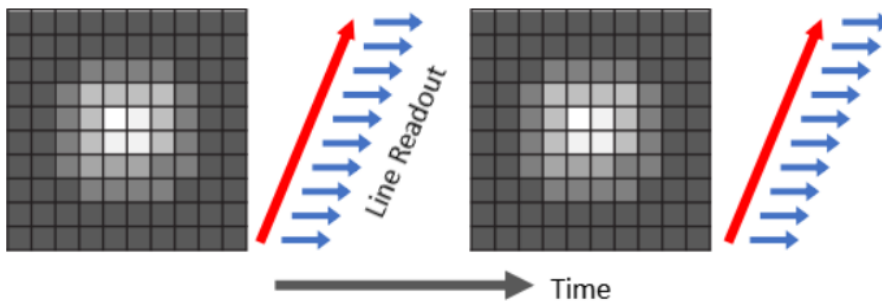


Figure 3-35 Schematic diagram of Up scanning

Down-up cycle: When scanning up and down, the rolling shutter starts at the top of the first row and goes down to the bottom of the last line. For the next frame, the rolling shutter will start at the bottom row and sweep up to the top first row, and so on. The image acquired in this mode is oriented in the same direction as the downward scan direction.

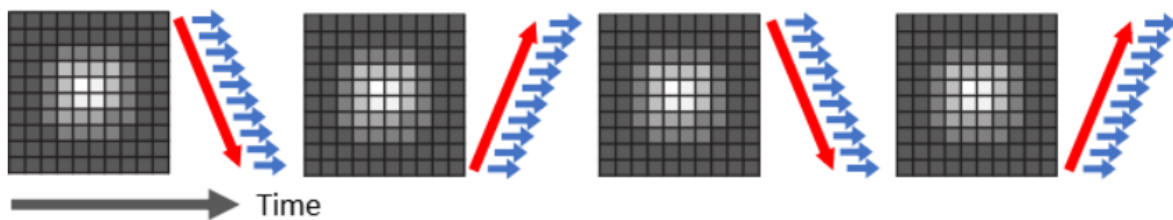


Figure 3-36 Schematic diagram of Down-up cycle scanning

3.17. Trigger Output

3.17.1. Hardware Trigger output circuit

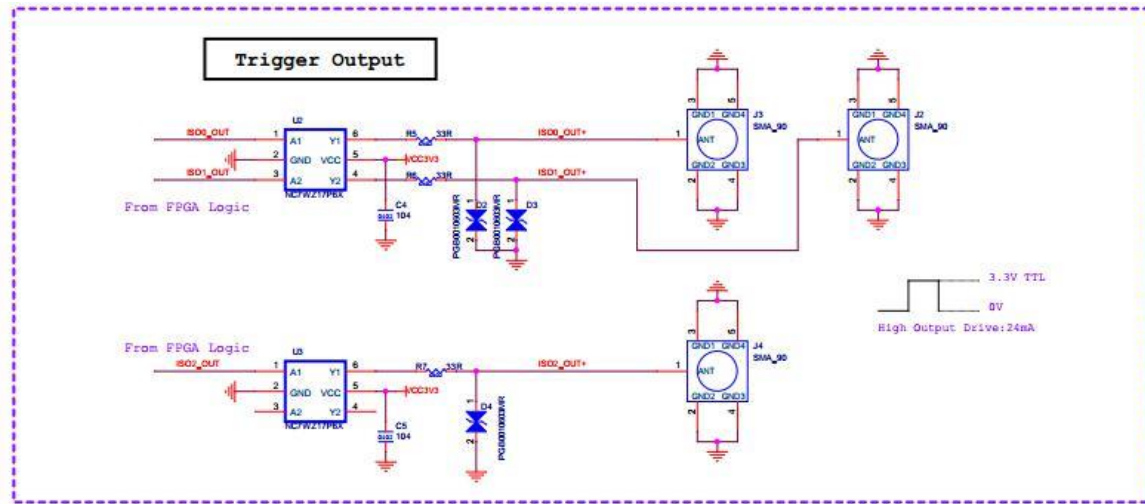


Figure 3-37

3.17.2. Trigger Output Timing Diagram

The camera has three external trigger output interfaces, each independently capable of outputting six timing signals. Each output signal can be independently configured on the three output ports and can simultaneously output to different devices.

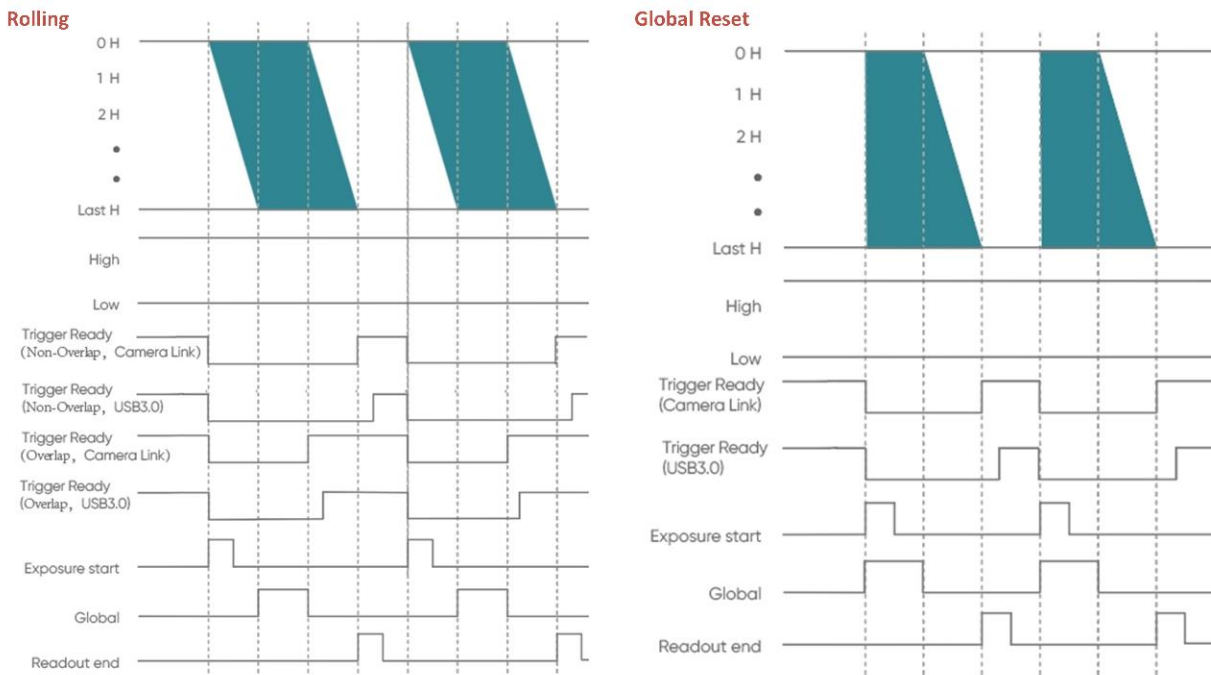


Figure 3-38 Trigger output timing diagram

- **High:** always output high level.

- **Low:** always output low level.
- **Trigger Ready:** when the camera is in the open-current state and can respond instantly to external triggers, the trigger ready output is high level.
- **Exposure Start:** output starting from the first line of exposure, the default pulse width is 5ms, which is customizable. And the output is in the TRIG.OUT3 interface by default.
- **Readout End:** output starting from the last line of exposure end, the default pulse width is 5ms, which is customizable. And the output is in the TRIG.OUT1 interface by default.
- **Global:** output from the beginning of the last line of exposure to the end of the first line of exposure end ([valid when the exposure time is larger than the readout time](#)), the default pulse width is 5ms, which is customizable. And the output is in the TRIG.OUT2 interface by default.

3.18. Cooling

Camera cooling effectively reduces "dark current noise" and the impact of hot pixels. The camera adopts semiconductor cooling using the Peltier effect, where an N-type and P-type material form a thermocouple. When a DC current is passed through the thermocouple, heating and cooling phenomena occur at the junctions due to the direction of the DC current. The cooling module is placed close to the chip to lower the chip's temperature and reduce dark current, while the hot end is connected to a metal heat sink to dissipate heat efficiently.

Both air cooling and water cooling are commonly used cooling methods. In air cooling, a fan exchanges excess heat with the surrounding air via airflow, while in water cooling, a liquid circulation system transfers excess heat. The Dhyana 400BSI V3 camera supports both air cooling and water cooling modes, allowing users to choose the appropriate cooling method based on the actual usage environment. In air cooling mode, the inlet and outlet vents are indicated as shown in the figure.

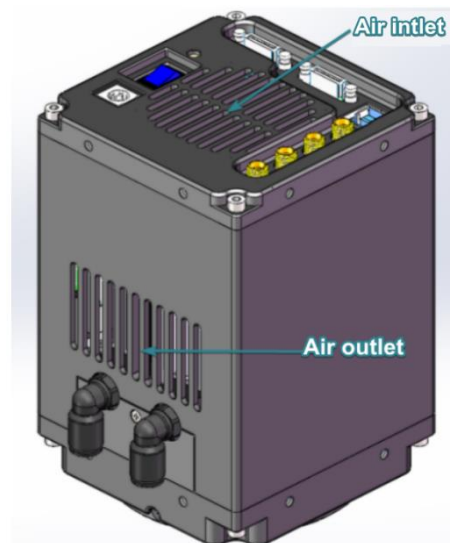


Figure 3-39 Schematic diagram of air inlet and outlet

Air cooling can achieve cooling effects of $\sim 35^{\circ}\text{C}$ below ambient temperature, while water cooling can achieve cooling effects of $\sim 45^{\circ}\text{C}$ below ambient temperature. The camera fan speed can be controlled variably, generally supporting High, Medium, and Low speed options. The higher the fan speed, the better the heat dissipation performance, while lower speeds result in lower vibration transmission. For complete low-vibration performance, the fan of the Dhyana 400BSI V3 camera can be completely turned off in the software, and a water cooling port is provided (refer to section 4.3 for installing water cooling).

4. Installation

4.1. Recommended computer configurations

Camera Interface	USB3.0	CameraLink
CPU	I5 and above performance, with a main frequency of 2.6GHz and above	
Operating system	Windows 10/11 64 bit PC	
Memory	8GB and above	
PCIe specifications	/	PCIe3.0*16

Note:

In CameraLink, sufficient bandwidth is required. If you see obvious image scrolling when opening the camera software, it is recommended to first confirm whether the bandwidth of the acquisition card is sufficient.

4.2. Camera installation

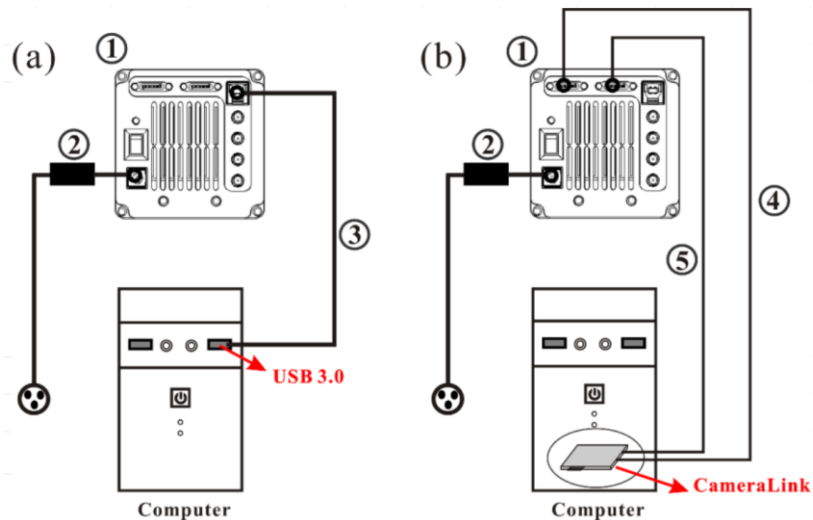


Figure 4-1 Dhyana 400BSI V3 camera connection diagram

- ① Dhyana 400BSI V3.0 camera
- ② Power adapter
- ③ USB 3.0 data cable
- ④ CameraLink cable 1

⑤ CameraLink cable 2

Connect one end of the USB 3.0 data cable or CameraLink data cable to the PC, and connect the USB to the USB 3.0 interface on the back of the host. Connect the other end to the sCMOS camera, lock the screw, then plug in the power cord, turn on the power switch, and you will see the indicator light lit up in red.

Note:

- 1) *To prevent the camera from overheating, do not cover the camera with cloth or any other material, nor block the camera's ventilation openings in any way.*
- 2) *If operating the camera in an enclosed environment, ensure there is at least a 10 cm gap between the camera's air intake and exhaust vents for safe operation and optimal cooling performance. If the camera is placed on a desk or platform, make sure the camera's vents are not facing downwards.*
- 3) *The depth of the C-mount is 7 mm. Over-tightening the base may scratch the glass surface.*
- 4) *Before connecting and disconnecting cables, please turn off the power to the camera and surrounding devices.*

4.3. Water cooling pipe installation

4.3.1. Connect the water cooling pipe

Operation steps:

- (1) Place the camera on a stable workbench;
- (2) Connect the water cooling pipe to the water pipe joint on the camera and make sure it is inserted in place, as shown in Figure 4-2 below;

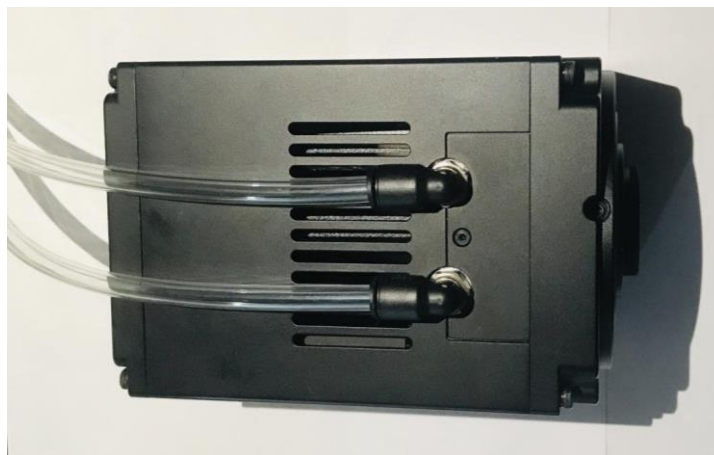


Figure 4-2

(3) Insert the water pipe into the water nozzle of the cooling water circulation machine and lock it with a clamp;

(4) The cooling water circulating machine water pipe is connected to the camera water pipe through an adapter valve.

4.3.2. Software Fan Status

(1) After installing the water cooling pipe, it is necessary to switch the cooling mode on the software. The default cooling method for the camera is air cooling, which can be switched to water cooling by adjusting the fan gear;

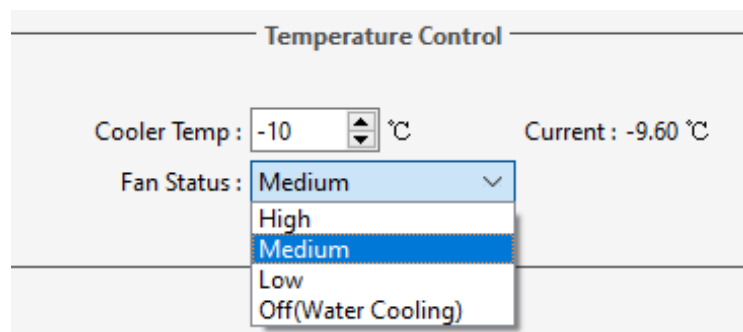


Figure 4-3

(2) If you choose to turn off the fan, the software will prompt you as follows. Click "Yes" to turn off the fan. Please ensure that the water cooling system is functioning properly before proceeding with this operation.

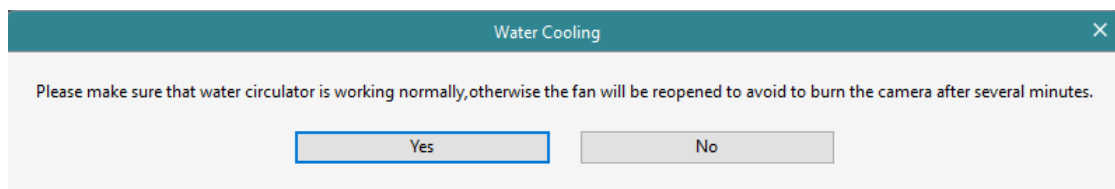


Figure 4-4

4.3.3. Disconnect the water cooling pipe

(1) Disconnect the power supply to the camera and all other equipment, including the recirculating water chiller;

(2) Following the instructions for the recirculating water chiller, unplug the water hose from the chiller and drain the water from the chiller;

(3) Press the adapter valve sleeve and remove the water hose from the recirculating water chiller to drain the internal water;

(4) Press the water connector and remove the camera's water hose from the hose connector. First,

position the side with the water valve facing sideways (**not upwards**). When removing the hose, ensure the water valve is facing downwards. Use an absorbent towel or paper towel to protect the area to ensure no water leaks into the camera.

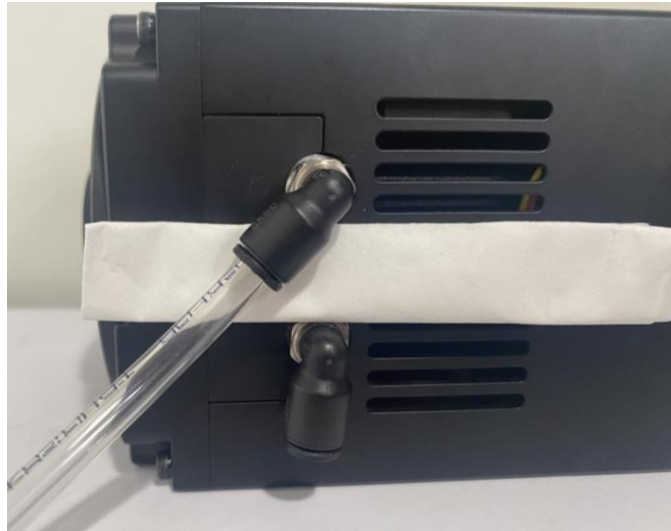


Figure 4-5 Removing water-cooled pipes

Note:

- 1) *Selection of cooling water: Deionized water is recommended;*
- 2) *Water temperature: Generally, a water temperature of 20°C is recommended. Inappropriate environmental conditions can cause condensation on the water valves and hoses, posing a risk of equipment damage. To ensure proper operation, the water temperature should not be below the dew point. Refer to the dew point table in the appendix for the dew point;*
- 3) *Pressure: The maximum water pressure entering the camera should not exceed 2 bar;*
- 4) *Recirculating water chiller: Use the chiller and cooling water correctly according to the chiller's instructions;*
- 5) *Properly install the water-cooling pipeline to ensure no leakage at the connections on both the camera and chiller ends;*
- 6) *Before operating the camera, ensure the correct installation of the recirculating water chiller and the camera's water valves, and that the water flow rate reaches 1L/min;*
- 7) *After operation, turn off the power to the camera and chiller, and drain the water from both the chiller and the camera.*

Warning:

- 1) **Do not turn off the recirculating water chiller during camera operation, as this may cause the chip to run at a high temperature continuously, leading to damage;**

2) *During camera operation, the water cooling and fan can be operated simultaneously, but they must not both be turned off simultaneously. At least one cooling method must be running to prevent the chip from running at high temperatures and being damaged.*

4.4. Frame grabber installation

Turn off the computer and open the cover of the computer host, as shown in Figure 4-6. Choose a PCIe slot with a transmission bandwidth greater than 850MB/s, insert the Frame grabber, secure it with screws, and then restart the computer. Connect the interface between the camera and the computer Frame grabber through a data transmission cable.

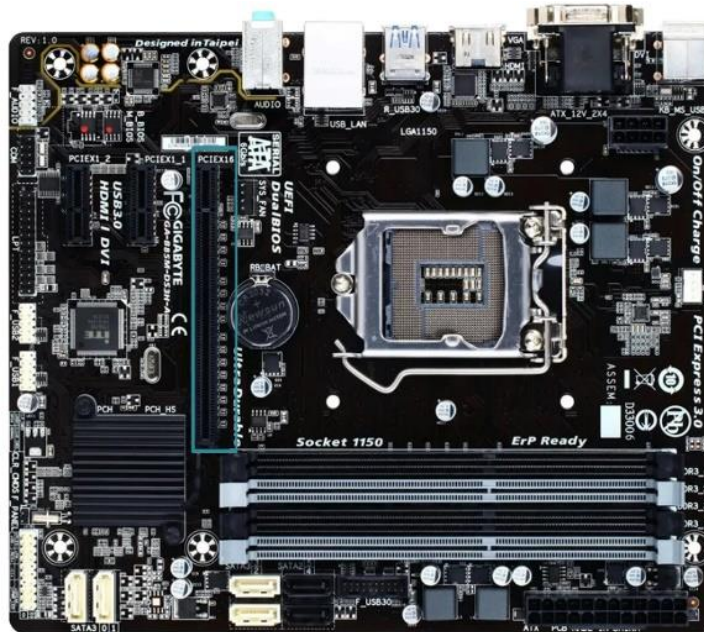


Figure 4-6 Computer motherboard diagram

Table 4-1 Maximum transfer rate corresponding to different PCIe slots

PCIe	X1	X4	X8	X16
1.0	250MB/s	1GB/s	2GB/s	4GB/s
2.0	500MB/s	2GB/s	4GB/s	8GB/s
3.0	985MB/s	3.9GB/s	7.8GB/s	15.7GB/s

Note:

- 1) *When installing and disassembling the Frame grabber, be sure to operate with power off;*
- 2) *When connecting the CamraLink cable, please operate with the camera power off and do not hot plug or unplug.*

4.5. Driver installation and uninstallation

This section will introduce the installation of camera USB driver, Frame grabber driver installation and uninstallation.

4.5.1. Camera USB driver installation

Operation steps:

- (1) Connect the camera to the computer and open the matching USB drive;
- (2) Double click to run the driver installation package;
- (3) Follow the prompts to click [Next] for default installation;

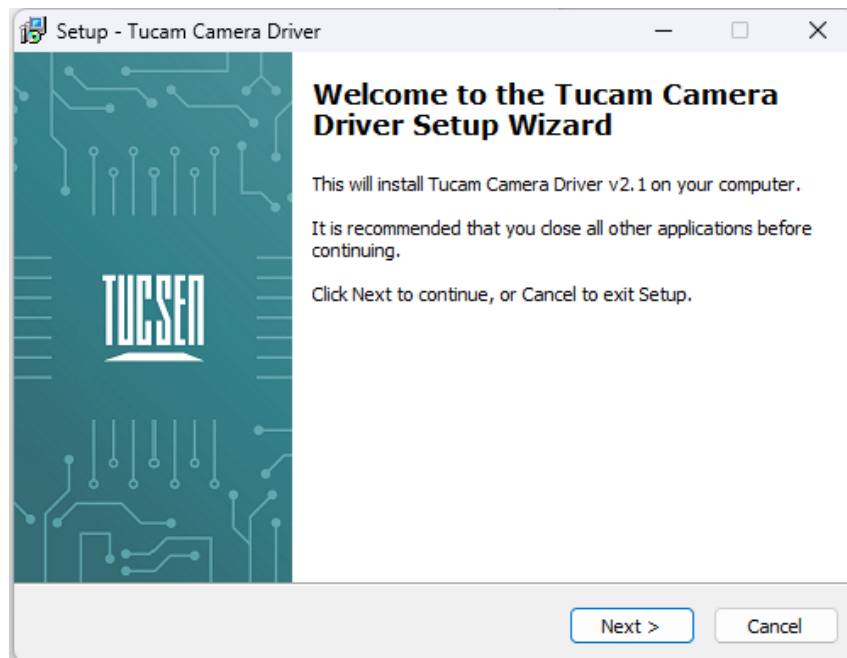


Figure 4-7

- (4) Selecting the contents of the installation, by default check the box to install Microsoft runtime libraries vcredist_2008 and vcredist_2013, unchecking the box may result in the software or third-party plug-ins not working;

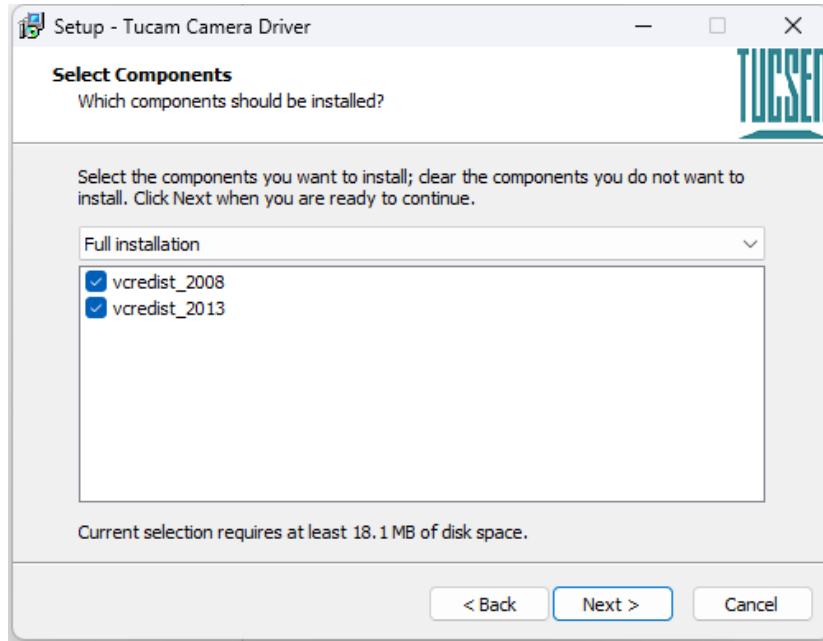


Figure 4-8

(5) Waiting for the driver installation to be completed;

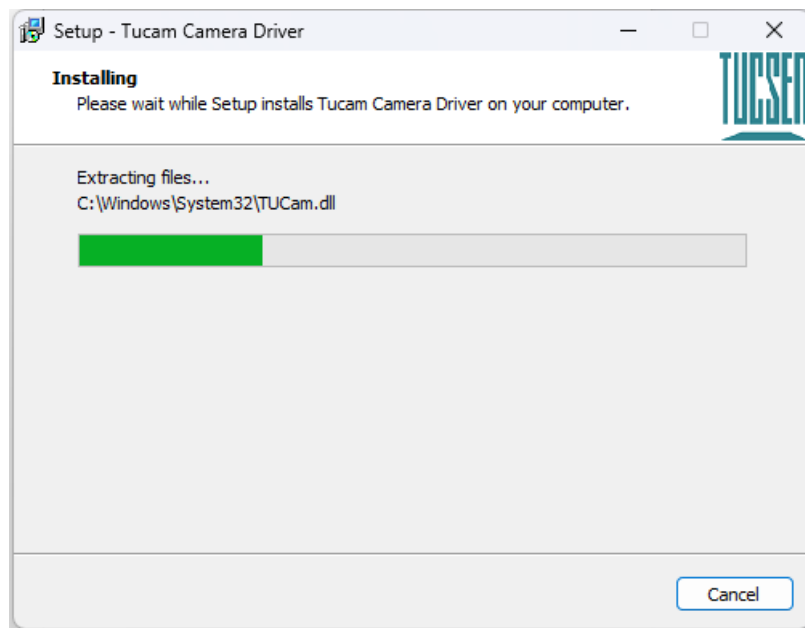


Figure 4-9

(6) Click "Finish" to complete the driver installation;

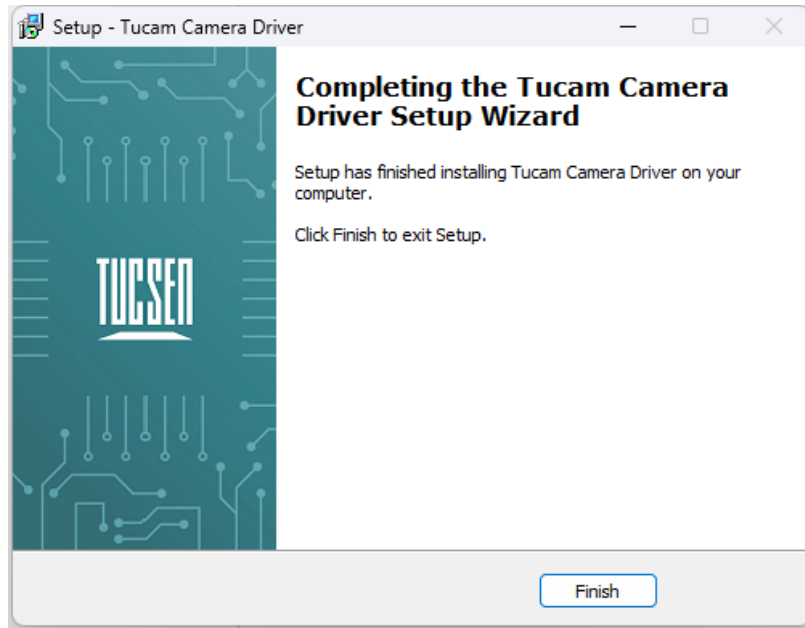


Figure 4-10

After installing the camera USB 3.0 driver, open the device manager on the computer. When the driver is successfully installed, the camera will appear under the image device without any yellow markings, as shown in the picture. If a yellow symbol appears, it indicates that the driver needs to be reinstalled.



Figure 4-11 Device Manager Display

4.5.2. CameraLink driver installation

Installation steps:

- (1) The camera is connected to the installed CameraLink Frame grabber CameraLink1 and CameraLink2 interfaces on the computer host through two CameraLink cables, and the interface sequence needs to be one-to-one corresponding;
- (2) Open the matching USB flash drive. Find the installation package for the acquisition card

driver;

(3) Double click to run the CameraLink acquisition card driver, follow the prompts to click [Next] for default installation, and finally click [Finish]. After restarting the computer host, the driver installation is completed.

(4) After the driver installation is completed, please restart the computer;

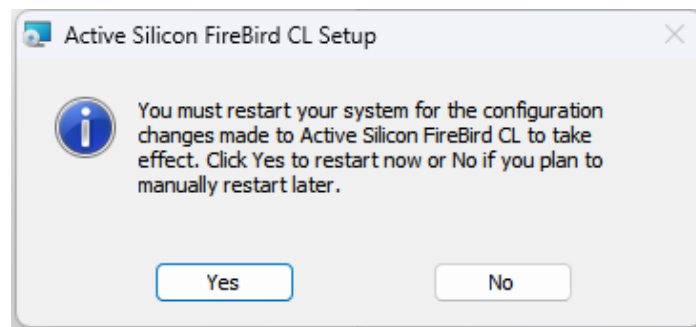


Figure 4-12

After installing the CameraLink driver, open the device manager on your computer. When the driver installation is successful, the CameraLink Frame grabber will appear in the device manager and display FireBird Baseboard. After connecting the camera, it will occupy the COM port, as shown in the following figure.

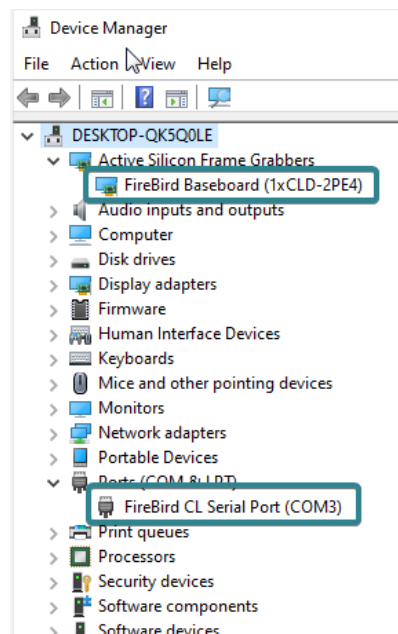


Figure 4-13

4.5.3. CameraLink driver uninstallation

Taking the Windows 11 system as an example, in the computer settings, click on Applications>Installed Applications, find Active Silicon FireBird CL, click on the three points on the right to uninstall, and follow the prompts to complete the uninstallation.

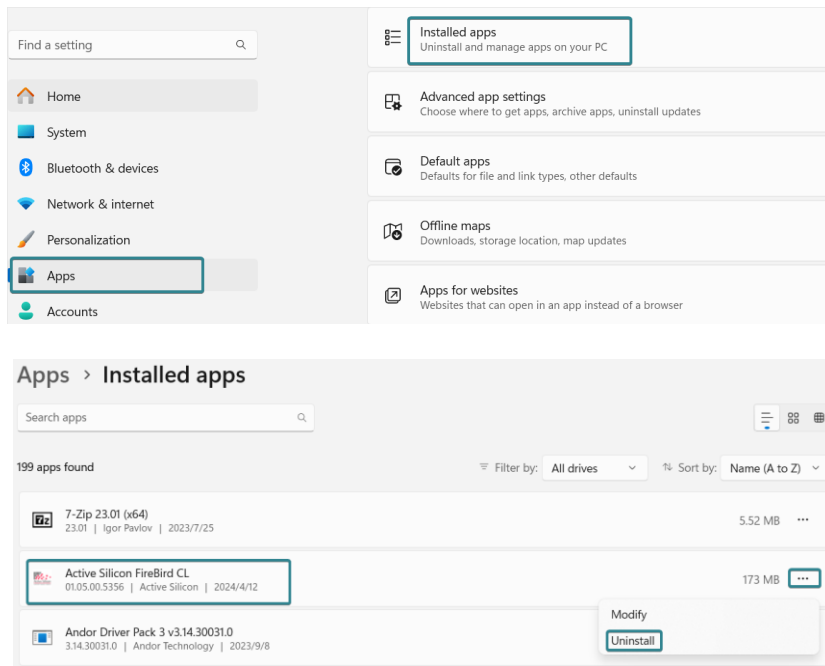


Figure 4-14

4.6. Software installation and uninstallation

4.6.1. Installation

Operation steps:

- (1) Open the supporting USB drive, double-click to run Mosaic V3 software;
- (2) Select the installation path, default to C drive, users can customize the installation path according to your needs;

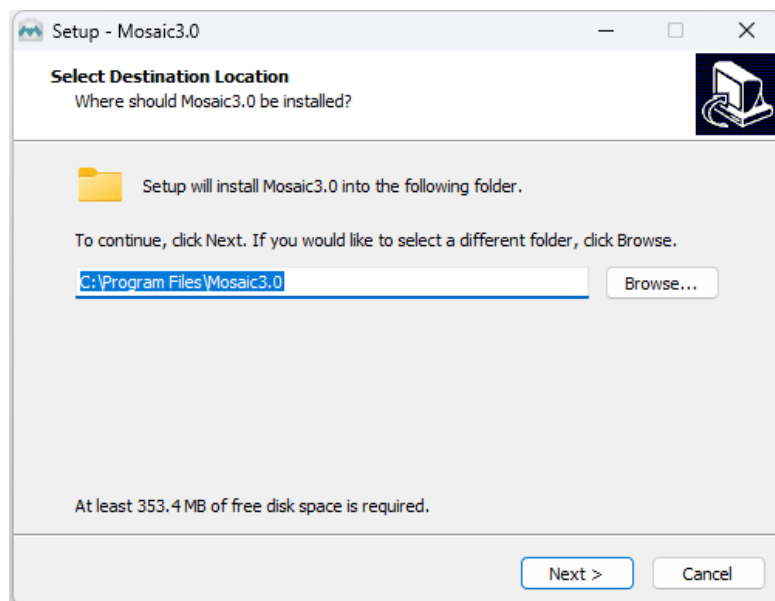


Figure 4-15

(3) Select the installation content. By default, select the option to install drivers and Microsoft runtime library vc-redist_2015, canceling the installation can result in the camera not being recognized by the software;

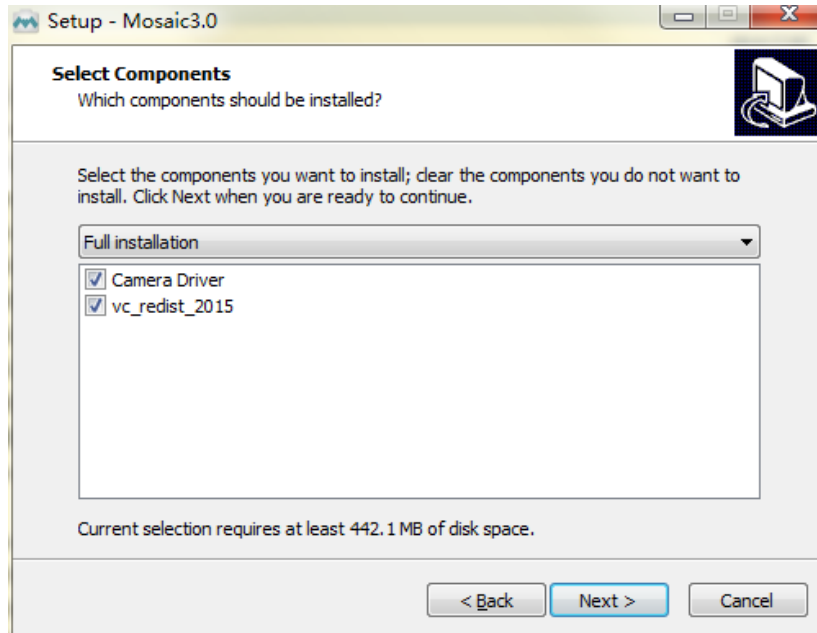


Figure 4-16

(4) Configure installation parameters and select whether to generate desktop shortcuts;

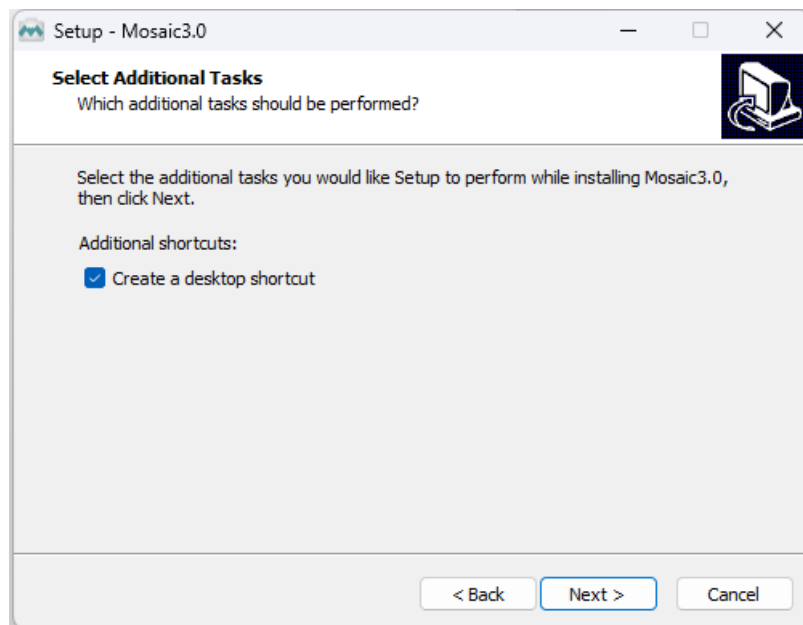


Figure 4-17

(5) After confirming all installation parameters, click "Install" to start executing the installation action;

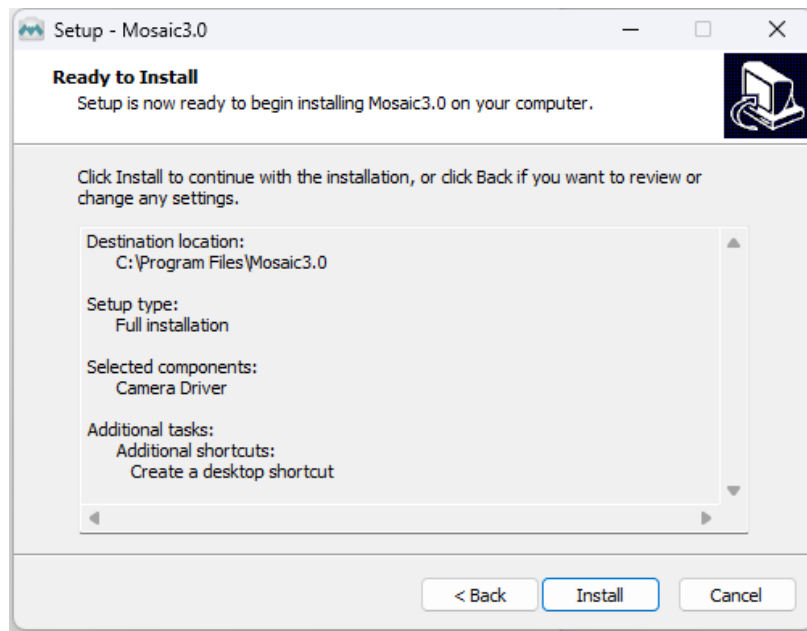


Figure 4-18

(6) Waiting for installation to complete;

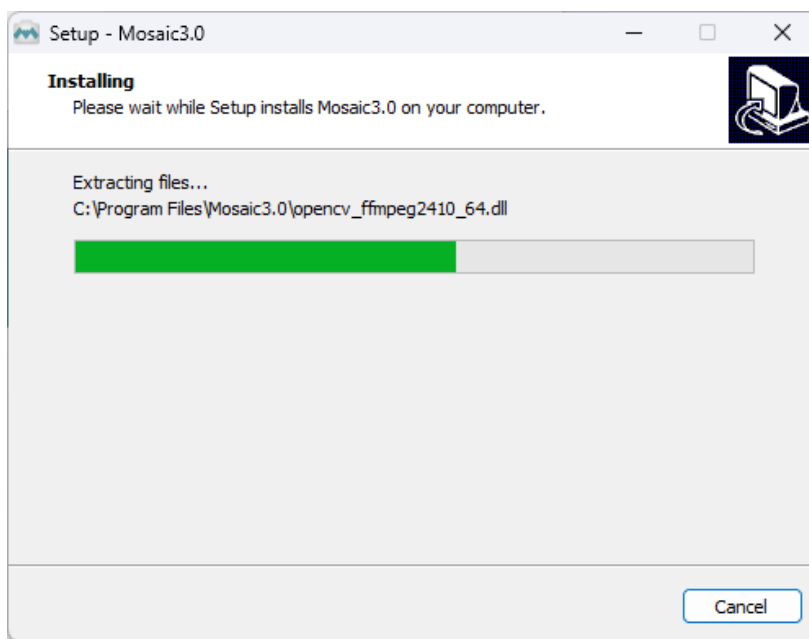


Figure 4-19

4.6.2. Uninstallation

There are three ways to uninstall Mosaic software:

(1) By uninstalling through the installation package, the existing version on the computer will be uninstalled when the installation package runs, and the default C drive path will take effect;

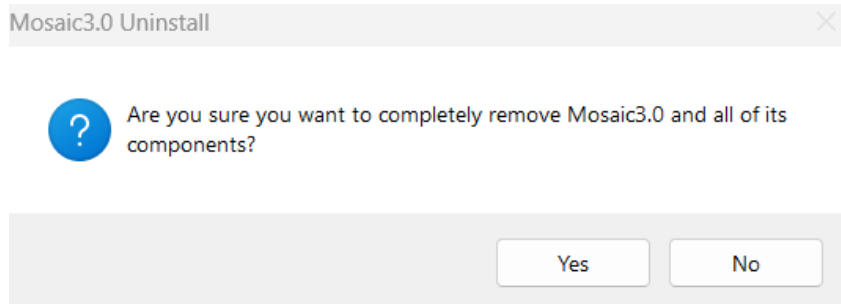


Figure 4-20 Uninstalling through installation package

(2) Under the installation path, find unins000.exe to uninstall, double-click uninstall;

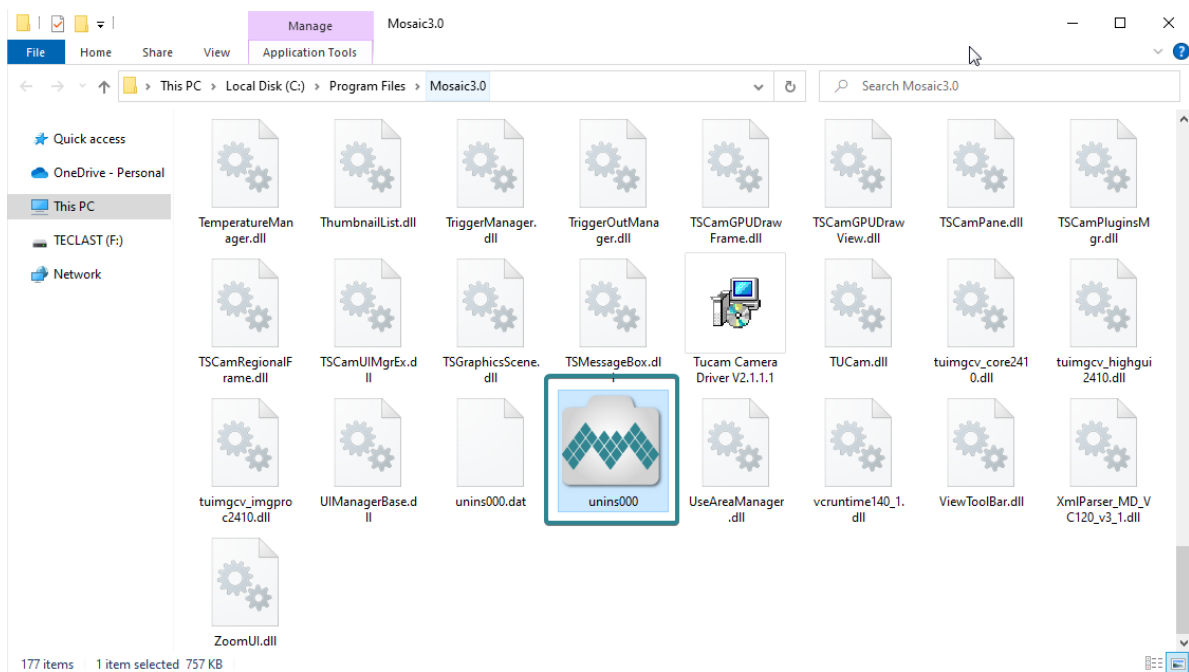


Figure 4-21

(3) Uninstall from the computer program management interface;

Note:

After uninstalling and reinstalling the software, all software configuration information and calibration table data will be deleted.

5. Maintenance

Damage caused by unauthorized maintenance or procedures will void the warranty.

5.1. Regular inspections

The product status should be regularly checked, especially the integrity of the external power supply and main cable, as well as the integrity of the power cord. Do not use damaged equipment.

5.2. Electrical safety inspection

- It is recommended to check the insulation and protective grounding integrity of the AC/DC converter every year
- Do not use damaged equipment

5.3. Cooling hoses and connectors

Users should regularly check all coolant hoses and connections for signs of leakage, damage, or wear. All seals must be intact before the camera system can be turned on, and any worn or damaged components must be replaced immediately.

5.4. Basic usage

- (1) Avoid opening the lens dust cover in dusty environments;
- (2) When opening the lens dust cover and installing the lens, keep the camera mouth facing downwards to prevent dust from falling on the surface of the windows;
- (3) When not in use for a long time, please keep the dust cover installed.

5.5. Window cleaning

When stains or spots are found in the images captured by the camera, please rule out whether the surface of the lens/microscope/objective at the camera interface is dirty.

If none of the above are true, it is certain that the camera itself brought it, and the window cleaning can be carried out according to the following steps:

- 1) Priority is given to the use of air blowing, the use of ear washing ball or air blowing off the general dust; together with the brush can remove most of the dust;

- 2) For stubborn oily dust, you need to prepare dust-free cotton swabs (or special mirror paper, non-woven fabric, etc.) and special tools such as anhydrous ethanol;
- 3) Use dust-free cotton swabs dipped in an appropriate amount of anhydrous ethanol to wipe along the surface of the window film, do not use too much force when wiping, and always in one direction, avoid back and forth wipe;
- 4) After wiping, use air blowers and other items to let the alcohol evaporate completely before continuing to use the window surface.

Note:

- 1) *If you cannot guarantee to complete the cleaning steps independently or do not have the required items, please be sure to contact us;*
- 2) *If the dirt still exists after following the above steps, try wiping again by following the above steps. If this does not solve the problem, consider that the chip is internally dirty. Please be sure to contact us at this time.*

6. Troubleshooting

6.1. The computer cannot recognize the camera

- 1) Confirm that the camera is powered on and turned on normally;
- 2) Confirm that the camera is connected to the computer normally;
- ① Confirm the connection sequence of the two cables through CameraLink connection;
- ② USB connection, please use the USB 3.0 interface on the backend of the desktop computer;
- 3) Confirm that the driver is working properly and check if the image device recognizes the camera in the computer device manager.

6.2. Software pauses or freezes

- 1) The computer may have turned on the energy-saving mode, the system CPU performance is reduced, resulting in the software can not work properly, there are dropped frames or software jamming and so on. You can check to ensure that the computer is in high-performance mode.
- 2) The computer has opened too many applications, resulting in the computer CPU occupation is too high, the software CPU utilisation is low and can not work properly. Can close the redundant applications.
- 3) Abnormal data cable connection, when the data cable is loose, or extended by the transfer too long will also lead to abnormal software connection, can not work properly.

6.3. The camera cannot reach the target cooling temperature

- 1) Confirm the ambient temperature, the maximum cooling temperature difference of the camera is $-45\text{ }^{\circ}\text{C}$ (water-cooled);
- 2) Confirm if the air outlet is blocked;
- 3) Confirm whether the fan rotates normally;
- 4) If water-cooling is used, make sure that the water-cooling cycle is functioning properly.

6.4. The frame rate cannot reach the nominal level

- 1) Confirm whether the exposure time affects the frame rate, and set the minimum exposure time to confirm the frame rate;

- 2) The frame rate in the table is the measured frame rate under ideal bandwidth, and the actual frame rate in the usage scenario will be affected by data transmission, which is related to the type of data interface used and the length of the transmission line;
- 3) Confirm that you are using the correct data transfer interface, USB requires a USB 3.0 interface, if you use a non-3.0 interface, the frame rate may not reach the nominal frame rate;
- 4) If you are using the USB3.0 interface but have switched to HUB/extension/expansion operations, it will also result in the inability to achieve the nominal frame rate;
- 5) For users who require high-speed image storage, if the frame rate cannot reach the nominal value using the CameraLink interface, it is necessary to check whether the bandwidth of the grabber card is limited/whether the recommended grabber card interface is used;
- 6) For users who require high-speed image storage, if the frame rate cannot reach the nominal value using the CameraLink interface, it is necessary to check whether the bandwidth of the acquisition card is limited/whether the recommended acquisition card interface is used.

7. FAQs

7.1. Why is the brightness of the captured image inconsistent with the preview window?

When using the camera for the first time and the target is dark, the software preview may show an all-black image. It is recommended to check Auto Left Scale (Auto Min) and Auto Right Scale (Auto Max) in the Histogram setting area, in which case the software preview will show the most suitable brightness and contrast. However, when you save the image, the default image saved by the software will not save the effect of auto colour gradation, resulting in inconsistency between the preview image and the captured image.

You can try the following solutions:

- 1) Disable the automatic colour gradation function of the software, the preview image will be consistent with the saved image;
- 2) Use professional image viewing tools such as ImageJ to open the tif image and adjust the colour gradation.
- 3) Use Mosaic V3 software to tick "Save the Adjusted Image" in the Capture section (can be used when you don't need the original image data value).

7.2. Stripe like flicker appears in the camera preview image

May be caused by an unsynchronised external light source. There may be a strobe light source in the environment, which can be judged by extending the exposure time. If it is an ambient light source, switching off the illumination source is sufficient. If from an irradiated sample light source, a regulated light source is required for illumination.

8. After-sales Support

1) Log in to the official website, click on the [Technical Support] module, and get answers to common questions.

2) Warranty:

- The quality assurance period starts from the date of shipment and lasts for a total of 24 months. During this period, any damage that meets the warranty requirements will be repaired free of charge;
- The warranty scope is limited to defects in product materials and manufacturing. Damage caused by self disassembly, water ingress, littering, or natural disasters is not covered by the warranty.

3) Contact professionals for technical support:





- TEL: +86-591-28055080-818
- Email: service@tucsen.com
- Visiting the official website to leave a message: <http://www.tucsen.com>

4) Please prepare the following information in advance:

- Camera model and S/N (product serial number);
- Software version number and computer system information;
- Description of the problem and any related images.

Appendix 1 : Dimensions

Unit: mm, Diameter: ϕ .

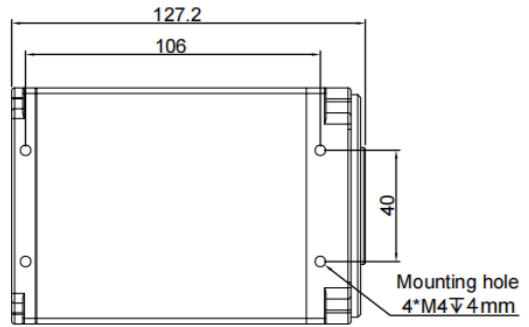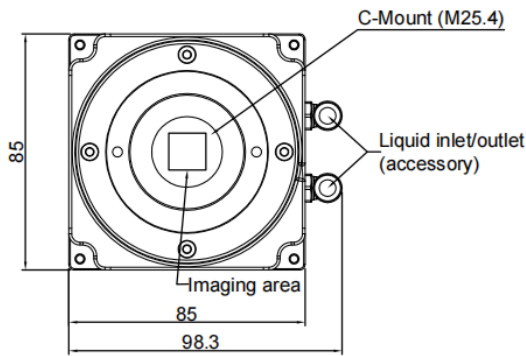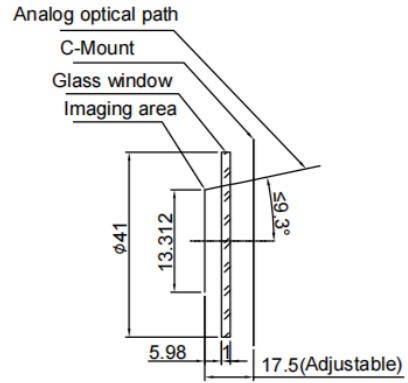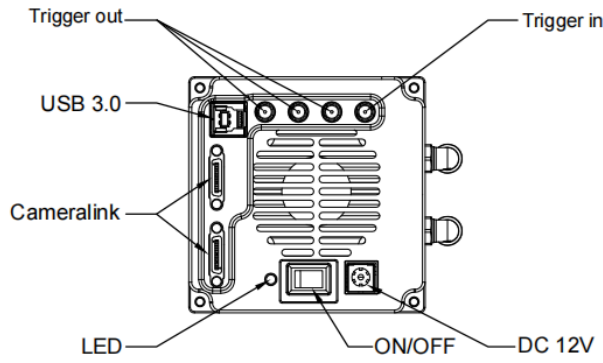

Appendix 2 : Specifications

Camera

Model	Dhyana 400BSI V3	
Sensor Type	BSI sCMOS	
Sensor Model	Gpixel GSENSE2020BSI	
Peak QE	95% @ 600 nm	
Color / Mono	Mono	
Array Diagonal	18.8 mm	
Effective Area	13.3 mm x 13.3 mm	
Resolution	2048 (H) x 2048 (V)	
Pixel Size	6.5 μm x 6.5 μm	
Full-Well Capacity	Typ. : 45 ke-	
Dynamic Range	Typ. : 90 dB	
Frame Rate	12bit firmware HDR: 43 fps @ CameraLink, 43 fps @ USB 3.0	11bit firmware HDR: 74 fps @ CameraLink, 45 fps @ USB 3.0
	High Speed: 100 fps @ CameraLink, 60fps @ USB 3.0	
Readout Noise	CMS(Typ.): 1.1 e- (Median) , 1.2 e- (RMS) HDR(Typ.): 1.6e- (Median) , 1.7 e- (RMS)	
Shutter Type	Rolling , Global Reset	
Exposure Time	11.2 μs ~ 10 s	
DSNU	0.2 e-	
PRNU	0.3 %	
Cooling Method	Air , Liquid	
Max. Cooling	45°C below ambient (Liquid)	
Dark Current	0.5 e-/pixel/s @-10°C	

Binning	2 x 2, 4 x 4
ROI	Support
Timestamp Accuracy	1 μ s
Trigger Mode	Hardware , Software
Output Trigger Signals	Exposure start, Global, Readout end, High level, Low level , Trigger ready
Trigger Interface	SMA
Data Interface	USB 3.0, CameraLink
Bit Depth	12 bit, 16 bit
Optical Interface	C-mount
Power Supply	12 V / 8 A
Power Consumption	45 W
Dimensions	85 mm x 85 mm x 127 mm
Weight	995 g
Software	Mosaic, SamplePro, LabVIEW, MATLAB, Micro-Manager2.0
SDK	C, C++, C#, Python
Operating System	Windows, Linux
Operating Environment	Temperature 0~40°C, Humidity 10~85%

Frame grabber

Brand	Active Silicon
Model	AS-FBD-1XCLD-2PE4-M
Operating System	Windows、Linux
Bus	PCIe 2x4, supports 2GB/s transfer from motherboard to computer
Transmission Speed	1.7 GB/s
Format	Half length PCI Express

Note: The parameters in this table are typical values and are subject to change without notice.



Appendix 3 : Third party software applications

Provide plugins for calling third-party software (LabVIEW, Matlab, Micro-Manager, etc.), please click on the link to download the configuration: [Tucsen camera software download – Tucsen](#)

Appendix 4 : Third party certification



Certificate of Compliance

Certificate No. : FQII-DZ-23009

Certificate Holder : Fujian Tucsen Photonics Co.,Ltd.

Address : Room E07, 1F of Comprehensive Building, NO.27 Jiayang Alley,
Antai Sub-District Gulou District, Fuzhou, Fujian

Product Description : Scientific Camera

Model Reference : Dhyana 400BSI V3

Brand Name : TUCSEN

Report No. : (2023)DZ10018

Standard/Directive :
EC Electromagnetic Compatibility Directive 2014/30/EU
EN 55032: 2015+A11:2020+A1:2020 , EN 55035: 2017+A11:2020 ,
EN IEC 61000-3-2:2019+A1:2021 , EN 61000-3-3:2013+A1:2019+A2:2021

This certificate applies specifically to the sample investigated in our test report number only. The test results apply only to the particular sample tested and to the specific tests carried out.

The CE marking can be affixed on the product after preparation of necessary conformity documentation.




Authorized Signatory
Date of Issue : Apr.06 , 2023



FUJIAN INSPECTION AND RESEARCH INSTITUTE FOR PRODUCT QUALITY
No. 121 Shantoujiao, West Yangqiao Road, Fuzhou, Fujian, P.R.China



验证报告

编号: CANEC2304333202

日期: 2023年04月14日 第1页,共26页

客户名称: 福建鑫图光电有限公司
客户地址: 福建省福州市鼓楼区安泰街道加洋路27号办公(档案)、综合楼1层E07室

样品名称: 科学级高灵敏相机
检测基本型号: Dh yana 400BSI V3
以上样品及信息由客户提供。

SGS工作编号: 23481722 - XM
样品接收日期: 2023年03月24日
验证周期: 2023年03月24日 - 2023年04月12日
验证要求: 参考欧盟RoHS指令2011/65/EU的修正指令(EU) 2015/863。
验证方法: 请参见后续页。
验证结果: 请参见后续页。

检测结果总结

检测项目	结论
欧盟RoHS指令2011/65/EU附录II修正指令(EU) 2015/863- 铅,汞,镉,六价铬,多溴联苯(PBBs),多溴二苯醚(PBDEs),邻苯二甲酸二丁酯(DBP),邻苯二甲酸丁苄酯(BBP),邻苯二甲酸二(2-乙基己基)酯(DEHP)和邻苯二甲酸二异丁酯(DIBP)	符合

通标标准技术服务有限公司广州分公司
授权签名

张鹰

Tyler Zhang 张鹰
批准签署人



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested.
Attention: To check the authenticity of testing/inspection report & certificate, please contact us at telephone: (86-755) 8387 9443, or email: CS.Support@sgs.com

SGS-China Inspection & Testing Services Co., Ltd.
Guangzhou Office (China) Laboratory

新加坡坡底路, 5000-25, Economic Technological Development Area, Guangzhou, Guangzhou, China 510663
中国·广东·广州高新技术产业开发区科学城科兴路118号 邮编: 510663

+ (86-20) 82158505 www.sgsgroup.com.cn
+ (86-20) 82158505 sgs.china@sgs.com

Member of the SGS Group (SGS SA)

Appendix 5 : Dew point table

		Humidity							
		20%	30%	40%	50%	60%	70%	80%	90%
Temperature	5							1.8	3.5
	6							2.8	4.5
	7						1.9	3.8	5.5
	8						2.9	4.8	6.5
	9					1.6	3.8	5.7	7.4
	10					2.6	4.8	6.7	8.4
	11					3.5	5.7	7.7	9.4
	12				1.9	4.5	6.7	8.7	10.4
	13				2.8	5.4	7.7	9.6	11.4
	14				3.7	6.4	8.6	10.6	12.4
	15			1.5	4.7	7.3	9.6	11.6	13.4
	16			2.4	5.6	8.2	10.5	12.6	14.4
	17			3.3	6.5	9.2	11.5	13.5	15.3
	18			4.2	7.4	10.1	12.4	14.5	16.3
	19		1.0	5.1	8.4	11.1	13.4	16.4	18.3
	20		1.9	6.0	9.3	12.0	14.4	16.4	18.3
	21		2.8	6.9	10.2	12.9	15.3	17.4	19.3
	22		3.6	7.8	11.0	13.9	16.3	18.4	20.3
	23		4.5	8.7	12.0	14.8	17.2	19.4	21.3
	24		5.4	9.6	12.9	15.8	18.2	20.3	22.3
25	0.5	6.2	10.5	13.9	16.7	19.1	21.3	23.2	
26	1.3	7.1	11.4	14.8	17.6	20.1	22.3	24.2	
27	2.1	8.0	12.3	15.7	18.6	21.1	23.3	25.2	
28	3.0	8.8	13.2	16.6	19.5	22.0	24.2	26.2	
29	3.8	9.7	14.0	17.5	20.4	23.0	25.2	27.2	

Appendix 6 : Update log

Version	Date	Modified Content
V1.0.0	2023-9-28	Create this document.
V1.0.1	2024-2-26	Adjustments have been made based on the new firmware version of the camera